



InSight PACS DICOM Conformance Statement
Version 2.12, Issue 3: Oct 2026

Enterprise PACS

Breast PACS

Disaster Recovery PACS

VNA

Author

Issue	Release Date	Reason for Change	Author	Approver
1	1 st June 2023	Update from Version 2.11	Stephen Davis	Shaun Ward
2	1 st Sept 2024	Update to Version 2.12	Stephen Davis	Shaun Ward
3	7 th Oct 2026	Rebranding from Version 2.12	Shaun Ward	Stephen Davis

1. Conformance Statement Overview

The InSight Enterprise PACS, Breast PACS, Disaster-Recovery PACS and Vendor-Neutral Archive (VNA) products share a common set of application components which constitute their DICOM interface to other systems. These components reside on the InSight Departmental Server system component; hence this Conformance Statement is versioned in accordance with the Departmental Server. Each product also contains a central database and various short-term and long-term storage nodes with which the DICOM components interact. Each may also contain other system components, but these are not relevant to this document.

- The InSight **Vendor-Neutral Archive** provides a self-contained system for archiving diagnostic medical images
- The InSight **Disaster-Recovery PACS** provides a diagnostic medical image archive with full PACS functionality available at short notice in the event of an institution losing access to its primary PACS
- The InSight **Breast PACS** provides a diagnostic medical image archive with fully integrated image viewing and reporting functionality and close integration with RIS and NBSS information systems, tailored to support Regional Breast Screening services
- The InSight **Enterprise PACS** provides a diagnostic medical image archive with fully integrated image viewing and reporting functionality, and close integration with an institution's EPR and RIS systems.

In all four products, external digital imaging systems which also conform to the relevant sections of the DICOM standard can connect to the InSight system to retrieve information about bookings (if the InSight system receives an appropriate external information feed), submit images for permanent storage, retrieve information about those stored images and retrieve the images themselves.

The InSight system may also connect to external systems to retrieve information about images that reside on those systems, and to request those images that it deems are required.

Table 3.1-1. Network Services.

Table 3.1-1 shows the DICOM Network services provided and used by the InSight components:

Table 3.1-1. Network Services.

SOP Classes	User of Service (SCU)	Provider of Service (SCP)
Transfer		
Computed Radiography Image Storage	Yes	Yes
Digital X-Ray Image Storage – For Presentation	Yes	Yes
Digital X-Ray Image Storage – For Processing	Yes	Yes
Digital Mammography X-Ray Image Storage – For Presentation	Yes	Yes
Digital Mammography X-Ray Image Storage – For Processing	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Presentation	Yes	Yes
Digital Intra-oral X-Ray Image Storage – For Processing	Yes	Yes
CT Image Storage	Yes	Yes
Ultrasound Multi-frame Image Storage (Retired)	Yes	Yes
Ultrasound Multi-frame Image Storage	Yes	Yes
MR Image Storage	Yes	Yes
MR Spectroscopy Storage	Yes	Yes
Nuclear Medicine Image Storage (Retired)	Yes	Yes
Ultrasound Image Storage (Retired)	Yes	Yes
Ultrasound Image Storage	Yes	Yes
Secondary Capture Image Storage	Yes	Yes
Multi-frame Single Bit Secondary Capture Image Storage	Yes	Yes
Multi-frame Greyscale Byte Secondary Capture Image Storage	Yes	Yes

Multi-frame Greyscale Word Secondary Capture Image Storage	Yes	Yes
Multi-frame True Colour Secondary Capture Image Storage	Yes	Yes
12-lead ECG Waveform Storage	Yes	Yes
General ECG Waveform Storage	Yes	Yes
Ambulatory ECG Waveform Storage	Yes	Yes
Hemodynamic Waveform Storage	Yes	Yes
Cardiac Electrophysiology Waveform Storage	Yes	Yes
Basic Voice Audio Waveform Storage	Yes	Yes
General Audio Waveform Storage	Yes	Yes
Arterial Pulse Waveform Storage	Yes	Yes
Respiratory Waveform Storage	Yes	Yes
Greyscale Softcopy Presentation State Storage	Yes	Yes
Colour Softcopy Presentation State Storage	Yes	Yes
Pseudo-Colour Softcopy Presentation State Storage	Yes	Yes
Blending Softcopy Presentation State Storage	Yes	Yes
X-Ray Angiographic Image Storage	Yes	Yes
X-Ray Radiofluoroscopic Image Storage	Yes	Yes
Breast Tomosynthesis Image Storage	Yes	Yes
Breast Projection X-Ray Image Storage - For Presentation	Yes	Yes
Breast Projection X-Ray Image Storage - For Processing	Yes	Yes
Intravascular Optical Coherence Tomography Image Storage - For Presentation	Yes	Yes
Intravascular Optical Coherence Tomography Image Storage - For Processing	Yes	Yes
Nuclear Medicine Image Storage	Yes	Yes
Raw Data Storage	Yes	Yes
Spatial Registration Storage	Yes	Yes
Spatial Fiducials Storage	Yes	Yes
Deformable Spatial Registration Storage	Yes	Yes
Surface Segmentation Storage	Yes	Yes
Tractography Results Storage	Yes	Yes
Real World Value Mapping Storage	Yes	Yes
Surface Scan Mesh Storage	Yes	Yes
Surface Scan Point Cloud Storage	Yes	Yes
VL Endoscopic Image Storage	Yes	Yes
Video Endoscopic Image Storage	Yes	Yes
VL Microscopic Image Storage	Yes	Yes
Video Microscopic Image Storage	Yes	Yes
VL Slide-Coordinates Microscopic Image Storage	Yes	Yes
VL Photographic Image Storage	Yes	Yes
Video Photographic Image Storage	Yes	Yes
Ophthalmic Photography 8 Bit Image Storage	Yes	Yes
Ophthalmic Photography 16 Bit Image Storage	Yes	Yes
Stereometric Relationship Storage	Yes	Yes
Ophthalmic Tomography Image Storage	Yes	Yes
Wide Field Ophthalmic Photography Stereographic Projection Image Storage	Yes	Yes
Wide Field Ophthalmic Photography 3D Coordinates Image Storage	Yes	Yes
Ophthalmic Optical Coherence Tomography En Face Image Storage	Yes	Yes
Ophthalmic Optical Coherence Tomography B-scan Volume Analysis Storage	Yes	Yes
VL Whole Slide Microscopy Image Storage	Yes	Yes
Lensometry Measurements Storage	Yes	Yes
Autorefractometry Measurements Storage	Yes	Yes
Keratometry Measurements Storage	Yes	Yes
Subjective Refraction Measurements Storage	Yes	Yes

Visual Acuity Measurements Storage	Yes	Yes
Spectacle Prescription Report Storage	Yes	Yes
Ophthalmic Axial Measurements Storage	Yes	Yes
Intraocular Lens Calculations Storage	Yes	Yes
Macular Grid Thickness and Volume Report Storage	Yes	Yes
Ophthalmic Visual Field Static Perimetry Measurements Storage	Yes	Yes
Ophthalmic Thickness Map Storage	Yes	Yes
Corneal Topography Map Storage	Yes	Yes
Basic Text SR	Yes	Yes
Enhanced SR	Yes	Yes
Comprehensive SR	Yes	Yes
Comprehensive 3d SR Storage	Yes	Yes
Extensible SR Storage	Yes	Yes
Procedure Log Storage	Yes	Yes
Mammography CAD SR Storage	Yes	Yes
Key Object Selection Storage	Yes	Yes
Chest CAD SR Storage	Yes	Yes
X-Ray Radiation Dose SR Storage	Yes	Yes
Radiopharmaceutical Radiation Dose SR Storage	Yes	Yes
Colon CAD SR Storage	Yes	Yes
Implantation Plan SR Storage	Yes	Yes
Acquisition Context SR Storage	Yes	Yes
Simplified Adult Echo SR Storage	Yes	Yes
Patient Radiation Dose SR Storage	Yes	Yes
Planned Imaging Agent Administration SR Storage	Yes	Yes
Performed Imaging Agent Administration SR Storage	Yes	Yes
Content Assessment Results Storage	Yes	Yes
Encapsulated PDF Storage	Yes	Yes
Encapsulated CDA Storage	Yes	Yes
Encapsulated STL Storage	Yes	Yes
Positron Emission Tomography Image Storage	Yes	Yes
RT Image Storage	Yes	Yes
RT Dose Storage	Yes	Yes
RT Structure Set Storage	Yes	Yes
RT Beams Treatment Record Storage	Yes	Yes
RT Plan Storage	Yes	Yes
RT Brachy Treatment Record Storage	Yes	Yes
RT Treatment Summary Record Storage	Yes	Yes
RT Ion Plan Storage	Yes	Yes
RT Ion Beams Treatment Record Storage	Yes	Yes
RT Physician Intent Storage	Yes	Yes
RT Segment Annotation Storage	Yes	Yes
RT Radiation Set Storage	Yes	Yes
C-Arm Photon-Electron Radiation Storage	Yes	Yes
Workflow Management		
Modality Worklist Information Model – FIND	No	Yes
Storage Commitment Push Model	Yes	Yes
Query/Retrieve		
Patient Root Query / Retrieve Information Model – FIND	Yes	Yes
Patient Root Query / Retrieve Information Model – MOVE	Yes	Yes
Study Root Query / Retrieve Information Model – FIND	Yes	Yes
Study Root Query / Retrieve Information Model – MOVE	Yes	Yes
Patient / Study Only Query/Retrieve Information Model – FIND (Retired)	Yes	Yes
Patient / Study Only Query/Retrieve Information Model – MOVE (Retired)	Yes	Yes

The InSight Components described in this document do not support any DICOM Media Services.



2. Contents

1.	Conformance Statement Overview	3
2.	Contents.....	6
3.	Introduction	11
3.1.	Audience	11
3.2.	Remarks	11
3.3.	Terms and Definitions	11
3.4.	Basics of DICOM Communication	12
3.5.	Abbreviations	13
3.6.	References	14
4.	Networking	15
4.1.	Implementation Model	15
4.1.1.	Application Data Flow.....	15
4.1.2.	Functional Definition of AEs	17
4.1.2.1.	Functional Definition of InList	17
4.1.2.2.	Functional Definition of InDigoX.....	17
4.1.2.3.	Functional Definition of InPort	17
4.1.2.4.	Functional Definition of InQuire	17
4.1.3.	Sequencing of Real-World Activities	18
4.2.	AE Specification.....	19
4.2.1.	Common Application Entity Association Policies	19
4.2.1.1.	Application Context Name	19
4.2.1.2.	Policy for Association Rejection or Abort during Negotiation	19
4.2.1.3.	Association Termination.....	20
4.2.2.	InList Application Entity Specification	21
4.2.2.1.	SOP Classes	21
4.2.2.2.	Association Policies	21
4.2.2.2.1.	General.....	21
4.2.2.2.2.	Number of Associations.....	21
4.2.2.2.3.	Asynchronous Nature	21
4.2.2.2.4.	Implementation Identifying Information	22
4.2.2.3.	Association Initiation Policy.....	22
4.2.2.4.	Association Acceptance Policy.....	22
4.2.2.4.1.	Activity: Imaging Device Issues Request for Modality Worklist Information	22

4.2.2.4.1.1.	Description and sequencing of Activities.....	22
4.2.2.4.1.2.	Accepted Presentation Contexts	22
4.2.2.4.1.3.	SOP Specific Conformance for Verification SOP Class.....	22
4.2.2.4.1.4.	SOP Specific Conformance for Modality Worklist Query SOP Class	23
4.2.3.	InDigoX Application Entity Specification	25
4.2.3.1.	SOP Classes	25
4.2.3.2.	Association Policies	27
4.2.3.2.1.	General.....	27
4.2.3.2.2.	Number of Associations.....	27
4.2.3.2.3.	Asynchronous Nature	28
4.2.3.2.4.	Implementation Identifying Information	28
4.2.3.3.	Association Initiation Policy.....	28
4.2.3.3.1.	Activity: Storage Commitment Notification over new Association	28
4.2.3.3.1.1.	Description and Sequencing of Activities	28
4.2.3.3.1.2.	Proposed Presentation Contexts.....	29
4.2.3.3.1.3.	SOP Specific Conformance for Storage Commitment SOP Class	29
4.2.3.4.	Association Acceptance Policy.....	30
4.2.3.4.1.	Activity: Receipt of SOP Instances and Storage Commitment Requests.....	30
4.2.3.4.1.1.	Description and sequencing of Activities.....	30
4.2.3.4.1.2.	Accepted Presentation Contexts	30
4.2.3.4.1.3.	SOP Specific Conformance for Verification SOP Class.....	31
4.2.3.4.1.4.	SOP Specific Conformance for Storage SOP Classes	31
4.2.3.4.1.5.	SOP Specific Conformance for Storage Commitment SOP Classes	32
4.2.3.4.2.	Activity: Receipt of IOCM KOS Object	33
4.2.3.4.2.1.	Description and Sequencing of Activities	33
4.2.3.4.2.2.	Accepted Presentation Contexts	33
4.2.3.4.2.3.	SOP Specific Conformance for Storage of IOCM KOS Object	33
4.2.4.	InPort Application Entity Specification.....	33
4.2.4.1.	SOP Classes	33
4.2.4.2.	Association Policies	34
4.2.4.2.1.	General.....	34
4.2.4.2.2.	Number of Associations.....	34
4.2.4.2.3.	Asynchronous Nature	34
4.2.4.2.4.	Implementation Identifying Information	34
4.2.4.3.	Association Initiation Policy.....	35

4.2.4.3.1.	Activity: InSight System Interrogates Remote System	35
4.2.4.3.1.1.	Description and Sequencing of Activities	35
4.2.4.3.1.2.	Patient Demographic Query.....	35
4.2.4.3.1.3.	Patient History Query	35
4.2.4.3.1.4.	Patient ID Query from Booking Reference	35
4.2.4.3.1.5.	Explicit Study Query	36
4.2.4.3.1.6.	Proposed Presentation Contexts.....	36
4.2.4.3.2.	SOP Specific Conformance for Patient Root and Patient/Study Only CFind	37
4.2.4.3.3.	SOP Specific Conformance for Study Root CFind	38
4.2.4.3.4.	Response Status Handling.....	39
4.2.4.3.5.	Activity: InSight System Requires Objects Residing on Remote System	40
4.2.4.3.5.1.	Description and Sequencing of Activities	40
4.2.4.3.5.2.	Proposed Presentation Contexts.....	40
4.2.4.3.5.3.	SOP Specific Conformance for Retrieve Service Classes	41
4.2.4.3.5.4.	Response Status Handling.....	41
4.2.4.3.5.5.	Sub-Operation Dependent Behaviour	42
4.2.4.4.	Association Acceptance Policy.....	42
4.2.5.	InQUIRE Application Entity Specification	42
4.2.5.1.	SOP Classes	42
4.2.5.2.	Association Policies	45
4.2.5.2.1.	General.....	45
4.2.5.2.2.	Number of Associations.....	45
4.2.5.2.3.	Asynchronous Nature	45
4.2.5.2.4.	Implementation Identifying Information	46
4.2.5.3.	Association Initiation Policy.....	46
4.2.5.3.1.	Activity: Storage of Composite Objects to Remote AE	46
4.2.5.3.1.1.	Description and Sequencing of Activities	46
4.2.5.3.1.2.	Proposed Presentation Contexts.....	46
4.2.5.3.1.3.	SOP Specific Conformance for Storage Service Classes	47
4.2.5.3.1.4.	Response Status Handling.....	48
4.2.5.3.2.	Activity: Initiate Storage Commitment (Push-Model) to Request Transfer of long-term ownership of Composite Objects to Remote AE	49
4.2.5.3.2.1.	Description and Sequencing of Activities	49
4.2.5.3.2.2.	Proposed Presentation Contexts.....	49
4.2.5.3.2.3.	SOP Specific Conformance for Storage Commitment SOP Class	49

4.2.5.3.3.	Activity: Send IOCM KOS Object	50
4.2.5.3.3.1.	Description and Sequencing of Activities	50
4.2.5.3.3.2.	Proposed Presentation Contexts.....	50
4.2.5.3.3.3.	SOP Specific Conformance for Storage of IOCM KOS Object	50
4.2.5.4.	Association Acceptance Policy.....	51
4.2.5.4.1.	Activity: Handling Query / Retrieve Requests and Storage Commitment Notifications from Remote AEs	51
4.2.5.4.1.1.	Description and sequencing of Activities.....	51
4.2.5.4.1.2.	Accepted Presentation Contexts	52
4.2.5.4.1.3.	SOP Specific Conformance for Verification Class.....	53
4.2.5.4.1.4.	SOP Specific Conformance for Query Service Classes.....	53
4.2.5.4.1.5.	SOP Specific Conformance for Retrieve Service Classes	55
4.2.5.4.1.6.	SOP Specific Conformance for Storage Commitment SOP Class	56
4.3.	Network Interfaces.....	57
4.3.1.	Physical Network Interface	57
4.3.2.	Additional Protocols	57
4.3.3.	IPv4 and IPv6	57
4.4.	Configuration	57
4.4.1.	AE Title / Presentation Address Mapping	57
4.4.1.1.	Local AE Titles	57
4.4.1.2.	Remote AE Title / Presentation Address Mapping.....	57
4.4.2.	Parameters	58
5.	Media Interchange	60
6.	Support of Character Sets.....	60
7.	Security	60
7.1.	Security Profiles	60
7.2.	Association Level Security	60
7.3.	Application Level Security	60
8.	Annexes.....	61
8.1.	IOD Contents.....	61
8.1.1.	Created SOP Instances.....	61
8.1.1.1.	Greyscale Softcopy Presentation State IOD Modules	61
8.1.1.2.	Colour Softcopy Presentation State IOD Modules	62
8.1.1.3.	Spatial Registration IOD Modules	62
8.1.1.4.	IOCM Rejected Image Note KOS IOD Modules	62

8.1.1.5.	Basic Text Structured Report IOD Modules	63
8.1.1.6.	Common Modules	63
8.1.1.7.	Presentation State Modules	64
8.1.1.8.	Spatial Registration Modules	69
8.1.1.9.	IOCM KOS Modules	72
8.1.1.10.	Basic Text Structured Report Modules	74
8.1.2.	Usage of Attributes from received IODs	76
8.1.3.	Attribute Mapping	78
8.1.4.	Coerced / Modified fields	79
8.2.	Data Dictionary of Private Attributes	80
8.3.	Coded Terminology and Templates	80
8.3.1.	Private Code Definitions	80

3. Introduction

3.1. Audience

This document is written for those who need to understand how the InSight Enterprise PACS, Breast PACS, Disaster Recovery PACS or VNA will integrate into their healthcare facility. This includes both those responsible for overall imaging network policy and architecture, and integrators who need to have a detailed understanding of the DICOM features of the products.

This document contains some basic DICOM definitions so that any reader may understand how these products implement DICOM features. However, integrators are expected to fully understand all the DICOM terminology, how the tables in this document relate to the products' functionality, and how that functionality integrates with other devices that support compatible DICOM features.

3.2. Remarks

The scope of this DICOM Conformance Statement is to facilitate integration between instances of the InSight VNA and PACS product families and other DICOM products. The Conformance Statement should be read and understood in conjunction with the DICOM Standard. DICOM by itself does not guarantee interoperability, however the Conformance Statement does facilitate a first-level comparison for interoperability between different applications supporting compatible DICOM functionality.

This Conformance Statement should not replace validation with other DICOM equipment to ensure proper exchange of intended information - the user should be aware of the following important issues:

- The comparison of different Conformance Statements is just the first step towards assessing interconnectivity and interoperability between these products and other DICOM conformant equipment
- Test procedures should be defined and executed to validate the required level of interoperability with specific compatible DICOM equipment, as established by the healthcare facility

3.3. Terms and Definitions

Informal definitions are provided in Table 3.3-1 for the following terms used in this Conformance Statement - the DICOM Standard is the authoritative source for formal definitions of these terms.

Table 3.3-1. Table of Terms.

Term	Description
Abstract Syntax	the information agreed to be exchanged between applications, generally equivalent to a Service/Object Pair (SOP) Class. Examples: Verification SOP Class, Modality Worklist Information Model Find SOP Class, Computed Radiography Image Storage SOP Class.
Application Entity (AE)	an end point of a DICOM information exchange - i.e. the software that sends or receives DICOM information objects or messages. A single device may have multiple Application Entities.
Application Entity Title	the externally known name of an <i>Application Entity</i> , used to identify a DICOM application to other DICOM applications on the network.
Application Context	the specification of the type of communication used between <i>Application Entities</i> . For all DICOM communication this is the DICOM network protocol.
Association	a network communication channel set up between <i>Application Entities</i> .
Attribute	a unit of information in an object definition; a data element identified by a <i>tag</i> . The information may be a complex data structure (sequence), itself composed of lower level data elements. Examples: Patient ID (0010,0020), Accession Number (0008,0050), Photometric Interpretation (0028,0004), Procedure Code Sequence (0008,1032).
Information Object Definition (IOD)	the set of <i>Attributes</i> that specify a class of data object. The <i>Attributes</i> may be specified as Mandatory (Type 1), Required but possibly unknown (Type 2), or Optional (Type 3). There may be conditions

	associated with the use of an Attribute (Types 1C and 2C). Examples: MR Image IOD, CT Image IOD, Print Job IOD.
Module	a set of <i>Attributes</i> within an <i>Information Object Definition</i> that are logically related to each other. Example: Patient Module includes Patient Name, Patient ID, Patient Birth Date, and Patient Sex.
Negotiation	first phase of <i>Association</i> establishment that allows <i>Application Entities</i> to agree on the types of data to be exchanged and how that data will be encoded.
Presentation Context	the set of DICOM network services used over an <i>Association</i> , as negotiated between <i>Application Entities</i> ; includes <i>Abstract Syntaxes</i> and <i>Transfer Syntaxes</i> .
Protocol Data Unit (PDU)	a packet of a DICOM message sent across the network. Devices must specify the maximum size packet they can receive for DICOM messages.
Presentation Data Value (PDV)	a message fragment conveyed in a P-DATA <i>PDU</i>
Security Profile	a set of mechanisms, such as encryption, user authentication, or digital signatures, used by an <i>Application Entity</i> to ensure confidentiality, integrity, and/or availability of exchanged DICOM data.
Service Class Provider (SCP)	role of an <i>Application Entity</i> that provides a DICOM network service; typically, a server that performs operations requested by another <i>Application Entity</i> (<i>Service Class User</i>).
Service Class User (SCU)	role of an <i>Application Entity</i> that uses a DICOM network service; typically, a client. Examples: imaging modality (image storage SCU, and modality worklist SCU), imaging workstation (image query/retrieve SCU).
Service/Object Pair (SOP) Class	the specification of the network transfer (service) of a particular type of data (object); the fundamental unit of DICOM interoperability specification. Examples: Ultrasound Image Storage Service, Basic Grayscale Print Management.
Service/Object Pair (SOP) Instance	an information object; a specific occurrence of information exchanged according to a <i>SOP Class</i> specification. Examples: a specific x-ray image.
Tag	a 32-bit identifier for a data element, represented as a pair of four digit hexadecimal numbers, the “group” and the “element”. If the “group” number is odd, the tag is for a private (manufacturer-specific) data element. Examples: (0010,0020) [Patient ID], (07FE,0010) [Pixel Data], (0019,0210) [private data element].
Transfer Syntax	the encoding used for exchange of DICOM information objects and messages. Examples: JPEG <i>compressed</i> (images), little endian explicit value representation.
Unique Identifier (UID)	a globally unique “dotted decimal” string that identifies a specific object or a class of objects; an ISO-8824 Object Identifier. Examples: Study Instance UID, SOP Class UID, SOP Instance UID.
Value Representation (VR)	the type of an individual DICOM data element, for example: text, integer, person name, code. DICOM information objects can be transmitted with either explicit identification of the type of each data element (Explicit VR), or not (Implicit VR); with Implicit VR, the receiving application must use a DICOM data dictionary to look up the format of each data element.

3.4. Basics of DICOM Communication

This section describes terminology used in this Conformance Statement for the non-specialist. The key terms used in the Conformance Statement are highlighted in *italics* below. This section is not a substitute for formal DICOM training, and it makes many simplifications about the meanings of DICOM terms.

Two *Application Entities* (devices) that want to communicate with each other over a network using the DICOM protocol must first agree on several things during an initial network “handshake” (*Negotiation*). One of the two devices must initiate an *Association* (a connection to the other device), and ask if specific services, information and encoding are supported by the other device.

DICOM specifies a number of network services and types of information objects, each of which is called an *Abstract Syntax* for the Negotiation. DICOM also specifies a variety of methods for encoding data, denoted *Transfer Syntaxes*. The Negotiation allows the initiating Application Entity to propose combinations of Abstract Syntax and Transfer Syntax to be used on the Association; these combinations are called *Presentation Contexts*. The receiving Application Entity accepts the Presentation Contexts it supports.

For each Presentation Context, the Association Negotiation also allows the devices to agree on *Roles* – which one is the *Service Class User* (SCU - client) and which is the *Service Class Provider* (SCP - server). Normally the device initiating the connection is the SCU, i.e., the client system calls the server, though for some services the SCP can initiate an Association with a client in order to send an Event Notification.

The Association Negotiation finally enables exchange of maximum network packet (*PDU*) size, security information, and network service options (called *Extended Negotiation* information).

The Application Entities, having negotiated the Association parameters, may now commence the exchange of data. Common data exchanges include queries for worklists and lists of stored images, transfer of image objects and analyses (structured reports), and sending images to film printers. Each exchangeable unit of data is formatted by the sender in accordance with the appropriate *Information Object Definition* and sent using the negotiated Transfer Syntax. There is a Default Transfer Syntax that all systems must accept, but it may not be the most efficient for some use cases. Each transfer is explicitly acknowledged by the receiver with a *Response Status* indicating success, failure, or that query or retrieve operations are still in process.

3.5. Abbreviations

A list of abbreviations is given in Table 3.5-1.

Table 3.5-1. List of abbreviations.

Abbreviation	Meaning	Abbreviation	Meaning
AE	Application Entity	AET	Application Entity Title
CR	Computed Radiography	CT	Computed Tomography
DICOM	Digital Imaging and Communications in Medicine	DX	Digital X-ray
GSDF	Grayscale Standard Display Function	GSPS	Grayscale Softcopy Presentation State
HL7	Health Level 7 Standard	IO	Intra-oral X-ray
IOCM	Imaging Object Change Management	IOD	Information Object Definition
IPv4	Internet Protocol version 4	IPv6	Internet Protocol version 6
ISO	International Organization for Standards	JPEG	Joint Photographic Experts Group
LUT	Look-up Table	MG	Mammography (X-ray)
MPPS	Modality Performed Procedure Step	MR	Magnetic Resonance Imaging
MSPS	Modality Scheduled Procedure Step	MTU	Maximum Transmission Unit (IP)
MWL	Modality Worklist	NBSS	National Breast Screening Service
NM	Nuclear Medicine	O	Optional (Key Attribute)
OP	Ophthalmic Photography	OSI	Open Systems Interconnection
PACS	Picture Archiving and Communication System	PDU	Protocol Data Unit
PET	Positron Emission Tomography	R	Required (Key Attribute)
RF	Radio-fluoroscopy	RIS	Radiology Information System
RT	Radiotherapy	SC	Secondary Capture
SCP	Service Class Provider	SCU	Service Class User
SOP	Service-Object Pair	SPS	Scheduled Procedure Step
SR	Structured Reporting	TCP/IP	Transmission Control Protocol/Internet Protocol
U	Unique (Key Attribute)	UL	Upper Layer

US	Ultrasound	VL	Visible Light
VR	Value Representation	XA	X-ray Angiography

3.6. References

- NEMA PS3 Digital Imaging and Communications in Medicine (DICOM) Standard, available free at <http://medical.nema.org/>
- IHE RAD TF IHE (Integrating the Healthcare Enterprise) Radiology Technical Framework, available free at https://www.ihe.net/resources/technical_frameworks/#radiology

4. Networking

4.1. Implementation Model

4.1.1. Application Data Flow

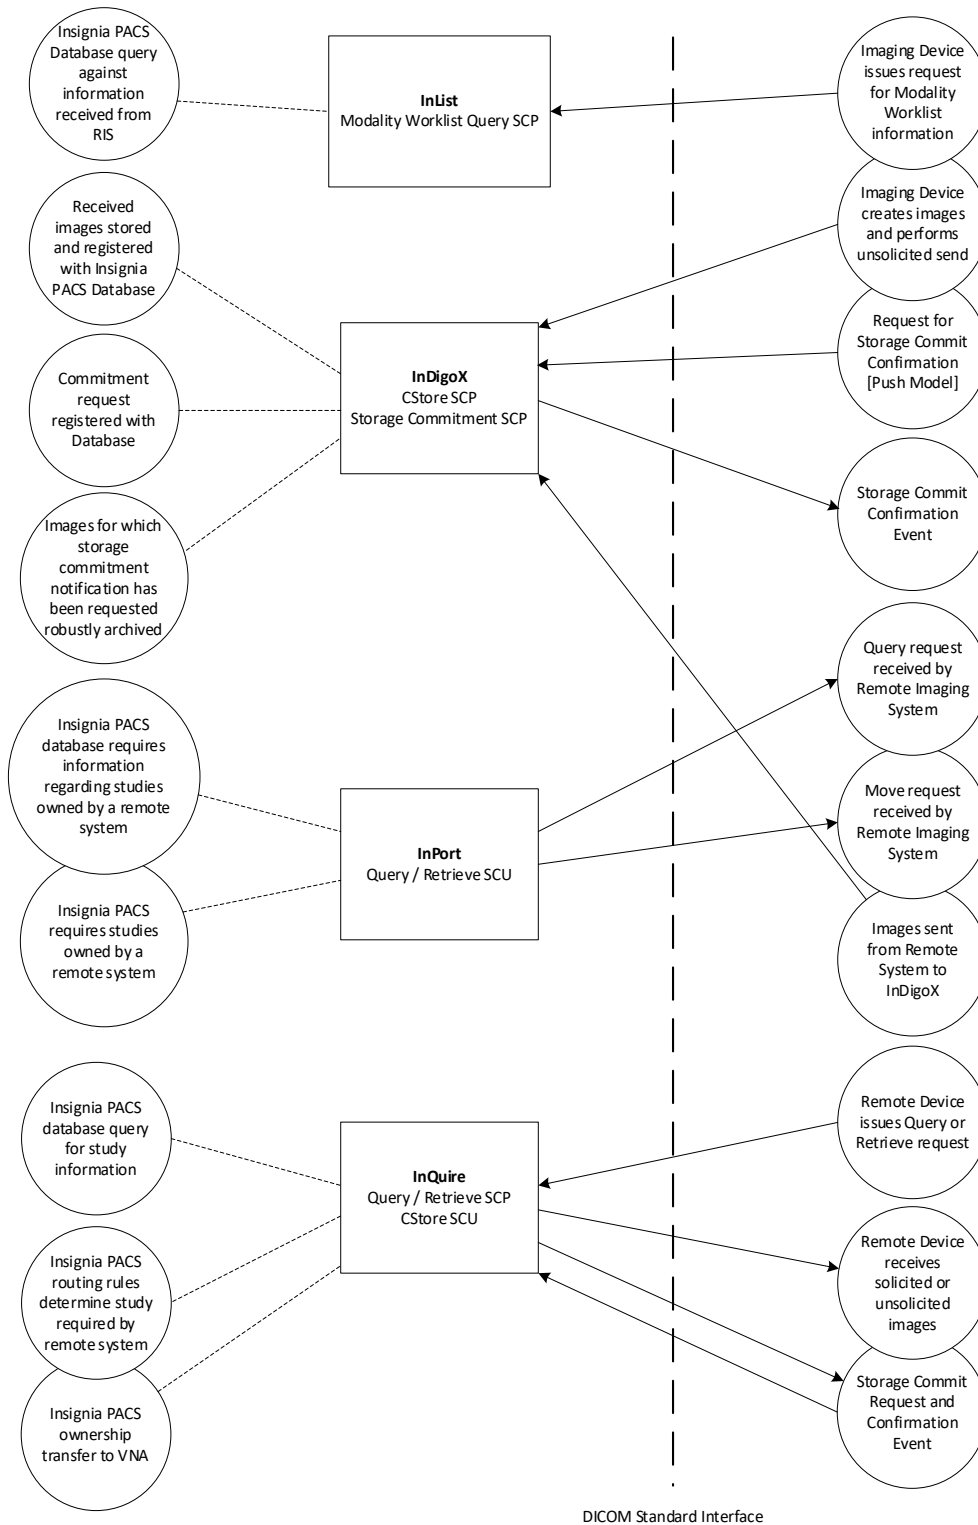


Figure 4.1-1. Insignia PACS DICOM Data Flow Diagram.

Each Departmental Server node in the InSight PACS has four distinct Application Entities, as shown in the Application Data Flow Diagram, **Figure 4.1-1**. These are implemented as Windows Services. Each Application Entity has a unique AE Title within the PACS environment and has a set of peer AE Titles from which and to which it will accept and request associations. Association requests from unknown AE Titles will be rejected.

- **InList** implements the Modality Worklist CFind service as an SCP. It handles an incoming Modality Worklist CFind request by performing a query against the InSight Database for booking details received by the InSight system from an institution's information system via an appropriate protocol such as HL7. If no such information feed exists, no results will be returned in the CFind response. InList will also respond to CEcho requests from known peer AEs.
- **InDigoX** implements the CStore service as an SCP for most common Storage SOP Classes. It also implements the Storage Commitment (Push Model) service as an SCP. When images are received, they are written to local storage, and the details are registered with the InSight database. When a Storage Commitment request is received, the SOP Instances requiring commit notification are noted in the database. When these SOP Instances are safely archived (the policy for this is determined by the institution but is typically that the image exists on two separate long-term storage nodes in the system), InDigoX will notify the remote device that the commitment request has been fulfilled. InDigoX will also respond to CEcho requests from known peer AEs.
- **InPort** implements the Query / Retrieve services as an SCU. If the InSight system wishes to interrogate a remote system for details of studies held for a certain patient, booking or date range, InPort will initiate a CFind request for the required data. If the InSight system determines that some of those studies are required, InPort will issue CMove requests for those studies, with the C-Move Destination set to the InDigoX AE Title.
- **InQuire** implements the Query / Retrieve services as an SCP and the Storage service as an SCU. It handles Query requests for Patient, Study, Series and Instance information, and also responds to C-Echo request as an SCP. When a Retrieve request is received, InQuire establishes a CStore association with the specified C-Move Destination AE and sends the SOP Instances itself. The InSight PACS products also have routing rules and user interactions that may result in InQuire sending unsolicited SOP Instances to a remote AE.
 - Where a separate DICOM long-term store (VNA) is utilised in the architecture, after routing a set of SOP Instances to the store, InQuire will issue a Storage Commitment request as SCU for those SOP Instances in order to transfer responsibility for the long-term storage of the objects to the remote system.
 - Where a separate DICOM long-term store (VNA) is utilised in the architecture, if objects are removed from a Study in the InSight System after any part of that Study has been sent to the long-term store, InQuire will generate an IOCM Rejection Note KOS Object and CStore it to the long term store, along with Replacement Instances as necessary, as described in the IHE Radiology Technical Framework Imaging Object Change Management Integration Profile.

4.1.2. Functional Definition of AEs

4.1.2.1. Functional Definition of InList

InList waits for another DICOM application to connect on the network socket configured for its Application Entity Title. It will accept Associations with Presentation Contexts for the DICOM Modality Worklist CFind Service Class and Verification Service Class. If the InSight system receives a suitable HL7 or other data feed from an external information system such as an Institution's RIS or NBSS, the response to a Modality Worklist query request will be generated from booking information held by the InSight Database.

4.1.2.2. Functional Definition of InDigoX

InDigoX waits for another DICOM application to connect on the network socket configured for its Application Entity Title. It will accept Associations with Presentation Contexts for SOP Classes of the Verification, Storage, and Storage Commitment (Push Model) Service Classes. Any images received on such Presentation Contexts will be written to Local Storage and registered with the InSight database. These images are then queued by the InSight system for copying to long-term storage nodes. Once robustly archived (the semantics of which depend on the Institution, but typically constitute an image being on two long-term storage nodes, or the subject of a successful Storage-Commitment by a separate DICOM Long-Term store), an image becomes a candidate for deletion from the Local Storage node as and when space is required for newly acquired images. The local storage node will typically have space for between six months and several years' worth of images, depending on the product's deployment details, and a SOP Instance can be expected to remain on local storage for this length of time.

If a Storage Commitment Push Model N-ACTION Request is received for images that reside on the Local Storage node, InDigoX will register the Transaction and SOP list with the InSight Database. The transaction is considered complete when all associated SOP Instances have been robustly archived as defined above. InDigoX polls the InSight database once a minute for completed Storage Commitment request transactions. When a transaction is complete, InDigoX will open a new association to the peer as the Storage Commitment SCP and send the N-EVENT-REPORT notification.

4.1.2.3. Functional Definition of InPort

InPort will instigate a Query association with a remote DICOM Application Entity when triggered to do so by user interaction or automated rules within the InSight system. The Query will be for the details of all Studies for a given Patient, for the Studies related to a specific booking, or for Studies within a specific date or time range. Once the study details have been retrieved, the InSight system will determine which studies are required, and InPort will initiate a Retrieve association with the remote DICOM Application Entity that was specified as the Retrieve AE in the query results for each given study. InPort will specify the InDigoX Application Entity Title as the C-Move Destination AE.

4.1.2.4. Functional Definition of InQuire

InQuire waits for another DICOM application to connect on the network socket configured for its Application Entity Title. InQuire will accept Associations with Presentation Contexts for SOP Classes of the DICOM Query-Retrieve Service Class and Verification Service Class, and also the Storage Commitment Push Model, where InQuire is acting as the SCU – see below. It will handle query and retrieve requests on these Presentation Contexts and respond with data objects with values corresponding to the contents of the InSight Database. For C-MOVE requests the destination for the image objects is determined from the Destination AE Title contained in the C-MOVE request. If this AE Title and its network address and port are known, InQuire will initiate an association with the C-MOVE

Destination AE with the required Storage Service Class Presentation Contexts determined from information held in the InSight Database for the SOP Instances in question.

The InSight PACS products (not the Vendor-Neutral Archive) also have automatic routing rules and user-initiated actions which may result in Inquire being triggered to send a set of SOP Instances to a remote DICOM Application Entity supporting the Storage Service Class as an SCP. Inquire will instigate an association with this AE, requesting Presentation Contexts for the required Storage Service Classes as determined from information held in the InSight Database for the SOP Instances in question.

Irrespective of why the association has been initiated, Inquire will update volatile demographic information in the SOP Instances being sent to the latest data received from the Institution Information system, if a suitable data feed exists. It will also convert the SOP Instances to the Transfer Syntax required for the accepted Presentation Context.

Where images have been routed to a separate long-term DICOM store, such as a VNA, Inquire will request Storage Commitment (Push Model) for all SOPs that are sent to that node. Once the Storage Commit complete N-EventReport for a Storage Commitment transaction is received (either on the same Association as the Storage Commitment N-Action request, or on a separate Association initiated by the storage node where Inquire is acting as the SCU for the Storage Commitment Presentation Context), the SOP instances that have been successfully committed will become deletable from the InSight PACS in due course.

When SOP Instances are removed from a study on the InSight System, where any part of that study has previously been sent to a separate long-term DICOM Store such as a VNA, Inquire will generate an IOCM Rejection Note KOS object and CStore it to the long-term DICOM Store, along with any replacement SOP Instances generated as part of the IOCM workflow. The KOS object and new Instances will then be the subject of a Storage Commitment request.

4.1.3. Sequencing of Real-World Activities

Within the real-world activities, the only sequencing constraint that a peer should observe is that SOP Instances must be C-Stored to InDigoX before a Storage Commitment request is made for them, and that Storage Commitment request should be made before the images have been deleted from the Local Storage node; however, deletion is unlikely to happen for at least 6 months after the C-Store event.

The InSight System guarantees that Inquire will only issue a Storage Commitment request after a successful CStore of the SOP instances concerned to the associated CStore SCP.

However, Inquire could generate an IOCM Rejection Note KOS object referencing SOP Instances that haven't yet been (or may never be) successfully stored to the recipient, as the IOCM KOS object will be sent if the recipient holds any part of an affected study. An IOCM KOS object will be sent whether or not a successful Storage Commitment notification has been received for any or all SOP Instances in the study.

4.2. AE Specification

4.2.1. Common Application Entity Association Policies

To prevent excessive duplication of information in this Conformance Statement and hence aid clarity, some details regarding Association Establishment and error handling which are common between all InSight Application Entities is detailed here and referenced from the specific Application Entity Specifications which follow.

4.2.1.1. Application Context Name

When establishing an association, the DICOM standard Application Context Name for DICOM 3.0 is always offered, and when accepting an association it is always accepted:

Table 4.2-1. DICOM Application Context.

Application Context Name	1.2.840.10008.3.1.1.1
--------------------------	-----------------------

4.2.1.2. Policy for Association Rejection or Abort during Negotiation

Each Application Entity which listens on its configured TCP/IP Port for an incoming network connection (InList, InDigoX and InQuire) has a configured list of remote Application Entities, together with their IP addresses and/or hostnames, from which it may accept connections. If a connection is detected from an IP address not in the configured list and not associated with any of the hostnames in the configured list, the first Association Request will result in the Association being Rejected with the reason “Calling AE Title Not Recognized”, and a message being logged with the InSight database. Subsequent connections from that IP address will result in the socket being closed immediately with no attempt at association negotiation.

If the IP Address is in the configured list, the Association negotiation will proceed, but will be rejected with the specified codes under the following circumstances (**Table 4.2-2**):

Table 4.2-2. Association Rejection Reasons.

Result	Source	Reason/Diag	Explanation
1: rejected, permanent	1: DICOM service-user UL	2: application context name not supported	The Association Request contained an unsupported Application Context Name. An Association Request with the same parameters will not succeed at a later time
1: rejected, permanent	1: DICOM service-user UL	3: calling AE title not recognized	The Association Request contained an unrecognized Calling AE Title. An Association Request with the same parameters will not succeed at a later time unless configuration changes are made. This rejection reason occurs when the Association Acceptor has not been configured to recognize the AE Title of the Association Initiator, or the Expected IP Addresses for the AE Title in question have been configured incorrectly
1: rejected, permanent	1: DICOM service-user UL	7: called AE title not recognized	The Association Request contained an unrecognized Called AE Title. An Association Request with the same parameters will not succeed at a later time. This rejection reason occurs when the Association Initiator is incorrectly configured and attempts to address the Association Acceptor using the wrong AE Title
1: rejected, permanent	2: DICOM service-provider (ACSE related function) UL	2: Protocol Version Not Supported	Bit zero of the Protocol-version field in the A-ASSOCIATE-RQ PDU is not set. An association Request with the same parameters will not succeed at a later time

2: rejected, transient	3: DICOM UL service-provider (Presentation related function)	2: local limit exceeded	The (configurable) maximum number of simultaneous Associations has been reached. An Association Request with the same parameters may succeed at a later time
------------------------	--	-------------------------	--

If the received data cannot be parsed as a valid A-ASSOCIATE-RQ PDU during Association Acceptance or as a valid A-ASSOCIATE-AC PDU during Association Initiation, an A-ABORT PDU will be sent with the following reasons (**Table 4.2-3**).

Table 4.2-3. Association Abort Reasons During Negotiation.

Source	Reason / Diag.	Explanation
0: DICOM UL service-user	n/a	Timeout occurred whilst waiting for data on the socket after at least one byte of the A-ASSOCIATE-RQ PDU has been received
1: DICOM UL service-provider	0: Reason not Specified	The PDU- or an Item-Field- Length was incorrect or inconsistent, hence parsing cannot be completed
1: DICOM UL service-provider	1: Unrecognized PDU	First byte received not 0x01, 0x02, 0x03, 0x04, 0x05, 0x06 or 0x07
1: DICOM UL service-provider	2: Unexpected PDU	First byte received not 0x01
1: DICOM UL service-provider	4: Unrecognized PDU parameter	Item-type byte not one of 0x10, 0x20, 0x21, 0x30, 0x40, 0x50 or 0x51 to 0xFF
1: DICOM UL service-provider	5: Unexpected PDU Parameter	Recognized Item-type not valid in the context it was received
1: DICOM UL service-provider	6: Invalid PDU Parameter Value	In an A-ASSOCIATE-AC PDU, either bit zero of the Protocol-version field is not set, or the Application Context name is not supported

If all Presentation Contexts in an Association Request are rejected, the Application Entity will respond with an A-ASSOCIATE-AC PDU, listing the reason for not accepting each Presentation Context. It is expected that the peer will then Release the Association immediately.

4.2.1.3. Association Termination

It is expected that the party which initiates the Association will under normal circumstances Release the Association in an orderly fashion when it has no further Commands to be performed or Events to notify.

If the InSight Application Entity is shutdown whilst an association is in progress, an A-RELEASE-RQ PDU will be issued.

If the InSight Application Entity encounters a protocol error during the exchange of P-DATA-TF PDUs or a response to a Release Request caused by Application shutdown is not received within 2500ms, an A-ABORT PDU will be issued, with the following reasons given (**Table 4.2-4**):

Table 4.2-4. Association Abort Reasons During Data Exchange.

Source	Reason / Diag.	Explanation
0: DICOM UL service-user	n/a	Timeout occurred after at least one byte of PDU has been received or no response to Release RQ after 2500ms during Application Entity shutdown
1: DICOM UL service-provider	1: Unrecognized PDU	First byte of PDU not 0x01, 0x02, 0x03, 0x04, 0x05, 0x06 or 0x07
1: DICOM UL service-provider	2: Unexpected PDU	First byte of PDU not 0x04, 0x05, or 0x07 (or 0x06 if Release RQ already sent)
1: DICOM UL service-provider	6: Invalid PDU Parameter Value	Presentation Context of the first received Presentation Data Value (PDV) fragment of a message was not accepted during negotiation

		• Presentation Context of a PDV which is not the first fragment of a message does not match the Presentation Context of the previous PDV • Failed to Parse a Command Set received over the Association
--	--	---

If an Abort PDU is received or the Network connection is lost, the InSight Application Entity will internally abort the current Command it is processing or has issued over the Association and log appropriate messages to the Application's Error Log. The resources related to the Association will be released and the Application Entity will await new Association requests or internal commands to initiate a new Association.

4.2.2. InList Application Entity Specification

4.2.2.1. SOP Classes

InList provides Standard Conformance to the following DICOM V3.0 SOP Classes (Table 4.2-5):

Table 4.2-5. SOP Classes for InList AE.

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	No	Yes
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	No	Yes

4.2.2.2. Association Policies

4.2.2.2.1. General

See **4.2.1 Common Application Entity Association Policies** for Application Context Name and Association Rejection and Termination policies.

InList will never initiate Associations; it continuously listens for Association Requests from external DICOM AE's. It will accept Associations for the Verification and Modality Worklist C-FIND services.

4.2.2.2.2. Number of Associations

The maximum number of simultaneous associations that InList will accept is configurable, and defaults to 5. There is no restriction within the configured limit for the maximum number of simultaneous associations acceptable from any given remote Application Entity.

Table 4.2-6. Number of Simultaneous Associations as an Association Acceptor for InList.

Maximum number of Simultaneous Associations	5 (Configurable)
---	------------------

4.2.2.2.3. Asynchronous Nature

The maximum number of asynchronous transactions that InList will allow to be invoked over a given association is 3.

Table 4.2-7. Asynchronous nature as an Association Acceptor for InList.

Maximum number of outstanding asynchronous transactions	3
---	---

4.2.2.2.4. Implementation Identifying Information

InList has the Implementation Class UID and Implementation Version Name specified in Table 4.2-8. The Implementation Version Name matches the version number of the InList executable, which is currently 2.0.1. All versions of InList in the 2.0.x.y family will adhere to this Conformance Statement.

Table 4.2-8. DICOM Implementation Class and Version for InList AE.

Implementation Class UID	1.2.826.0.1.3867976.7.108
Implementation Version Name	2.0.x.y

4.2.2.3. Association Initiation Policy

InList does not initiate Associations

4.2.2.4. Association Acceptance Policy

4.2.2.4.1. Activity: Imaging Device Issues Request for Modality Worklist Information

4.2.2.4.1.1. Description and sequencing of Activities

When InList accepts an Association with a Presentation Context for a supported SOP Class, the remote Application Entity can send any number of CEcho or Modality Worklist CFind requests to which InList will respond as appropriate; the remote Application Entity should release the Association when no further commands are to be sent. When processing a CFind request, the resulting InSight Database query will run to completion before any normal responses are sent; depending on the specified Matching Keys, some queries will take longer than others. If a C-CANCEL-FIND-RQ is received while the Database Query is in progress, a response with the status Cancelled will be sent immediately; the association can then be released or another CFind request sent as required by the SCU.

4.2.2.4.1.2. Accepted Presentation Contexts

InList will accept Presentation Contexts for the Abstract Syntax / Transfer Syntax combinations listed in **Table 4.2-9**. Note that all Transfer Syntaxes are acceptable for the Verification SOP Class as there is no Information Object associated with the Service. Where multiple Transfer Syntaxes are offered in a Presentation Context for a given Abstract Syntax in the Association Request, the first supported Transfer Syntax will be selected for that Presentation Context.

Table 4.2-9. Accepted Presentation Contexts by InList

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	Any		SCP	None
Modality Worklist Information Model - FIND	1.2.840.10008.5.1.4.31	Implicit Little Endian	1.2.840.10008.1.2	SCP	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

Note: Modality Worklist CFind Extended Negotiation - InList supports fuzzy semantic matching on Person Name

4.2.2.4.1.3. SOP Specific Conformance for Verification SOP Class

InList provides standard conformance to the Verification SOP Class as an SCP.

4.2.2.4.1.4. SOP Specific Conformance for Modality Worklist Query SOP Class

InList supports matching on the keys listed in Table 4.2-10 of which those marked (*) are Optional according to the Modality Worklist Information Model definition in Table K.6-1 of the DICOM Standard (PS 3.4-K.6.1.2.2).

Fuzzy semantic Person Name matching is performed on Patient Name and Scheduled Performing Physician Name using Microsoft SQL Server soundex functionality. This matching is also case-insensitive. If the Specific Character Set attribute (0008,0005) is present in the Query Data Set and set to Unicode UTF-8 (ISO_IR 192), Patient Name and Scheduled Performing Physician Name will be converted to ISO Latin 1 if possible. In all other cases the Character Set is ignored and these strings are assumed to be ISO Latin 1. In the Result Set the Specific Character Set attribute will be set to Latin 1 (ISO_IR 100) if and only if either Scheduled Performing Physician Name or Patient Name contain a character outside the ASCII Default repertoire.

Table 4.2-10. InList Modality Worklist Query Supported Matching Keys

Description	Tag	Remark
Scheduled Procedure Step Sequence	(0040,0100)	
> Scheduled Station AE	(0040,0001)	
> Scheduled Procedure Step Start Date	(0040,0002)	
> Scheduled Procedure Step Start Time	(0040,0003)	
> Modality	(0008,0060)	
> Scheduled Performing Physician Name	(0040,0006)	Case Insensitive Fuzzy Matching
> Scheduled Procedure Step Location	(0040,0011)	*
> Scheduled Procedure Step Status	(0040,0020)	*
Requested Procedure Priority	(0040,1003)	*
Accession Number	(0008,0050)	*
Patient Name	(0010,0010)	Case Insensitive Fuzzy Matching
Patient ID	(0010,0020)	Single Value Matching

InList will include the return key attributes in **Table 4.2-11** when they are present in the query request. The semantic governing the presence of data for Type 2 and Conditional fields is specified. Requests for matching on attributes not in this table will result in a warning status in the C-Find response.

Table 4.2-11. InList Modality Worklist Query Return Keys

Description	Tag	Return Type	Remark
Scheduled Procedure Step			
Scheduled Procedure Step Sequence	(0040,0100)	1	One Item will be returned
> Scheduled Station AE	(0040,0001)	1	
> Scheduled Procedure Step Start Date	(0040,0002)	1	
> Scheduled Procedure Step Start Time	(0040,0003)	1	
> Modality	(0008,0060)	1	
> Scheduled Performing Physician's Name	(0040,0006)	2	Populated if known
> Scheduled Procedure Step Description	(0040,0007)	1C	Always populated, value matches Protocol Code SQ > Code Meaning
> Scheduled Station Name	(0040,0010)	2	Always empty
> Scheduled Procedure Step Location	(0040,0011)	2	Populated if known
> Scheduled Protocol Code Sequence	(0040,0008)	1C	Always populated with one Item
>> Code Value	(0008,0100)	1	

>> Coding Scheme Designator	(0008,0102)	1	"INSIGHT PRIVATE" or as configured for Institution
>> Coding Scheme Version	(0008,0103)	3	Always empty
>> Code Meaning	(0008,0104)	3	Will match SPS Description
> Pre-Medication	(0040,0012)	2C	Always empty
> Scheduled Procedure Step ID	(0040,0009)	1	
> Requested Contrast Agent	(0032,1070)	2C	Always empty
> Scheduled Procedure Step Status	(0040,0020)	3	"SCHEDULED" or "ARRIVED"
Requested Procedure			
Requested Procedure ID	(0040,1001)	1	
Requested Procedure Description	(0032,1060)	1C	Always populated, value matches Procedure Code SQ > Code Meaning
Requested Procedure Code Sequence	(0032,1064)	1C	Always populated with one Item
> Code Value	(0008,0100)	1	
> Coding Scheme Designator	(0008,0102)	1	"INSIGHT PRIVATE" or as configured
> Coding Scheme Version	(0008,0103)	3	Always empty
> Code Meaning	(0008,0104)	3	Will match RQP Description
Study Instance UID	(0020,000D)	1	
Referenced Study Sequence	(0008,1110)	2	Always empty
Requested Procedure Priority	(0040,1003)	2	Always populated
Patient Transport Arrangements	(0040,1004)	2	Always empty
Requested Procedure Comments	(0040,1400)	3	
Names of Intended Recipients of Results	(0040,1010)	3	Zero or One value will be returned
Imaging Service Request			
Accession Number	(0008,0050)	2	Always populated
Requesting Physician	(0032,1032)	2	Populated if known
Referring Physician's Name	(0008,0090)	2	Populated if known
Requesting Service	(0032,1033)	3	
Visit Identification			
Admission ID	(0038,0010)	2	Populated if known
Visit Status			
Current Patient Location	(0038,0300)	2	Populated if known
Visit Relationship			
Referenced Patient Sequence	(0008,1120)	2	Always empty
Patient Identification			
Patient Name	(0010,0010)	1	
Patient ID	(0010,0020)	1	
Other Patient IDs	(0010,1000)	3	Zero or One value will be returned
Patient Demographic			
Patient DOB	(0010,0030)	2	Always populated
Patient Sex	(0010,0040)	2	Always populated
Patient's Weight	(0010,1030)	2	Always empty
Confidentiality constraint on patient data	(0040,3001)	2	Always empty
Patient Age	(0010,1010)	3	Calculated from DOB
Patient Address	(0010,1040)	3	Populated If Known
Patient Comments	(0010,4000)	3	
Patient Medical			
Patient State	(0038,0500)	2	Always empty
Pregnancy Status	(0010,21C0)	2	Always empty
Medical Alerts	(0010,2000)	2	Always empty
Contrast Allergies	(0010,2100)	2	Always empty
Special Needs	(0038,0050)	2	Always empty

InList will return the following statuses in the course of handling a Modality Worklist CFind request:

Table 4.2-12. InList Modality Worklist Query Response Status Reasons.

Service Status	Further Meaning	Error Code	Reasons
Failure	Identifier Does Not Match SOP Class	A900	The Identifier was missing or could not be interpreted as a Modality Worklist Information Object
	Unable to Process	C000	The InSight Database query to retrieve the worklist matches failed. Full details will be logged in the InList error log. Error Comment (0000,0902) will read "Failed to process Modality Worklist Query"
Cancelled	Matching terminated due to Cancel Request	FE00	The Cancelled status will be set on the next response returned after receiving the Cancel Request
Success	Matching is complete	0000	All Pending matches have been sent
Pending	Matches are continuing – all requested Optional Keys were supported	FF00	Response contains an Information Object representing the match containing all requested keys
	Matches are continuing – Warning that one or more Optional Keys were not supported	FF01	Response contains an Information Object representing the match, but some requested optional keys were not supported - these are logged in the InList error log

The handling of terminal communication errors and normal Association release are detailed in section 4.2.1.3 **Association Termination.**

4.2.3. InDigoX Application Entity Specification

4.2.3.1. SOP Classes

InDigoX provides Standard Conformance to the following DICOM V3.0 SOP Classes:

Table 4.2-13. SOP Classes for InDigoX AE.

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	No	Yes
Storage Commitment Push Model	1.2.840.10008.1.20.1	No	Yes
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	No	Yes
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	No	Yes
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	No	Yes
Digital Mammography XRay Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	No	Yes
Digital Mammography XRay Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	No	Yes
Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	No	Yes
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	No	Yes
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	No	Yes
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	No	Yes
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	No	Yes
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	No	Yes
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	No	Yes
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	No	Yes
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	No	Yes
Multi-frame Greyscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	No	Yes
Multi-frame Greyscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	No	Yes
Multi-frame True Colour Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	No	Yes

12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	No	Yes
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	No	Yes
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	No	Yes
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	No	Yes
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	No	Yes
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	No	Yes
General Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.2	No	Yes
Arterial Pulse Waveform Storage	1.2.840.10008.5.1.4.1.1.9.5.1	No	Yes
Respiratory Waveform Storage	1.2.840.10008.5.1.4.1.1.9.6.1	No	Yes
Greyscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	No	Yes
Colour Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	No	Yes
Pseudo-Colour Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	No	Yes
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	No	Yes
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	No	Yes
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	No	Yes
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	No	Yes
Breast Projection X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.13.1.4	No	Yes
Breast Projection X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.13.1.5	No	Yes
Intravascular Optical Coherence Tomography Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.14.1	No	Yes
Intravascular Optical Coherence Tomography Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.14.2	No	Yes
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	No	Yes
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	No	Yes
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	No	Yes
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	No	Yes
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	No	Yes
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	No	Yes
Tractography Results Storage	1.2.840.10008.5.1.4.1.1.66.6	No	Yes
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	No	Yes
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	No	Yes
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	No	Yes
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	No	Yes
Video Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1.1	No	Yes
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	No	Yes
Video Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2.1	No	Yes
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	No	Yes
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	No	Yes
Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	No	Yes
Ophthalmic Photography 8 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.1	No	Yes
Ophthalmic Photography 16 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.2	No	Yes
Stereometric Relationship Storage	1.2.840.10008.5.1.4.1.1.77.1.5.3	No	Yes
Ophthalmic Tomography Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.4	No	Yes
Wide Field Ophthalmic Photography Stereographic Projection Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.5	No	Yes
Wide Field Ophthalmic Photography 3D Coordinates Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.6	No	Yes
Ophthalmic Optical Coherence Tomography En Face Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.7	No	Yes
Ophthalmic Optical Coherence Tomography B-scan Volume Analysis Storage	1.2.840.10008.5.1.4.1.1.77.1.5.8	No	Yes
VL Whole Slide Microscopy Image Storage	1.2.840.10008.5.1.4.1.1.77.1.6	No	Yes
Lensometry Measurements Storage	1.2.840.10008.5.1.4.1.1.78.1	No	Yes
Autorefractive Measurements Storage	1.2.840.10008.5.1.4.1.1.78.2	No	Yes
Keratometry Measurements Storage	1.2.840.10008.5.1.4.1.1.78.3	No	Yes
Subjective Refraction Measurements Storage	1.2.840.10008.5.1.4.1.1.78.4	No	Yes
Visual Acuity Measurements Storage	1.2.840.10008.5.1.4.1.1.78.5	No	Yes
Spectacle Prescription Report Storage	1.2.840.10008.5.1.4.1.1.78.6	No	Yes
Ophthalmic Axial Measurements Storage	1.2.840.10008.5.1.4.1.1.78.7	No	Yes
Intraocular Lens Calculations Storage	1.2.840.10008.5.1.4.1.1.78.8	No	Yes
Macular Grid Thickness and Volume Report Storage	1.2.840.10008.5.1.4.1.1.79.1	No	Yes
Ophthalmic Visual Field Static Perimetry Measurements Storage	1.2.840.10008.5.1.4.1.1.80.1	No	Yes

Ophthalmic Thickness Map Storage	1.2.840.10008.5.1.4.1.1.81.1	No	Yes
Corneal Topography Map Storage	1.2.840.10008.5.1.4.1.1.82.1	No	Yes
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	No	Yes
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	No	Yes
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	No	Yes
Comprehensive 3d SR Storage	1.2.840.10008.5.1.4.1.1.88.34	No	Yes
Extensible SR Storage	1.2.840.10008.5.1.4.1.1.88.35	No	Yes
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	No	Yes
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	No	Yes
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	No	Yes
Chest CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.65	No	Yes
X-Ray Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.67	No	Yes
Radiopharmaceutical Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.68	No	Yes
Colon CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.69	No	Yes
Implantation Plan SR Storage	1.2.840.10008.5.1.4.1.1.88.70	No	Yes
Acquisition Context SR Storage	1.2.840.10008.5.1.4.1.1.88.71	No	Yes
Simplified Adult Echo SR Storage	1.2.840.10008.5.1.4.1.1.88.72	No	Yes
Patient Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.73	No	Yes
Planned Imaging Agent Administration SR Storage	1.2.840.10008.5.1.4.1.1.88.74	No	Yes
Performed Imaging Agent Administration SR Storage	1.2.840.10008.5.1.4.1.1.88.75	No	Yes
Content Assessment Results Storage	1.2.840.10008.5.1.4.1.1.90.1	No	Yes
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	No	Yes
Encapsulated CDA Storage	1.2.840.10008.5.1.4.1.1.104.2	No	Yes
Encapsulated STL Storage	1.2.840.10008.5.1.4.1.1.104.3	No	Yes
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	No	Yes
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	No	Yes
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	No	Yes
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	No	Yes
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	No	Yes
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	No	Yes
RT Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6	No	Yes
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	No	Yes
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	No	Yes
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	No	Yes
RT Physician Intent Storage	1.2.840.10008.5.1.4.1.1.481.10	No	Yes
RT Segment Annotation Storage	1.2.840.10008.5.1.4.1.1.481.11	No	Yes
RT Radiation Set Storage	1.2.840.10008.5.1.4.1.1.481.12	No	Yes
C-Arm Photon-Electron Radiation Storage	1.2.840.10008.5.1.4.1.1.481.13	No	Yes

4.2.3.2. Association Policies

4.2.3.2.1. General

See **4.2.1 Common Application Entity Association Policies** for Application Context Name and Association Rejection and Termination policies.

InDigoX can both initiate Associations and listen for Association Requests from Remote AEs. It will accept Associations for Verification, Storage and Storage Commitment Push Model Services. It will propose Associations only for the Storage Commitment Push Model Service, proposing the SCP role.

4.2.3.2.2. Number of Associations

The maximum number of simultaneous associations that InDigoX will accept is configurable, and defaults to 5. Unless configured otherwise, the maximum number of simultaneous associations acceptable from any given remote Application Entity is half the configured overall maximum. InDigoX may at any time initiate a single Association for Storage Commitment N-EVENT-REPORT notification irrespective of how many other Associations it is currently handling.

Table 4.2-14. Number of Simultaneous Associations for InDigoX.

Maximum number of simultaneous requested Associations	5 (Configurable)
Maximum number of simultaneous proposed Associations	1

4.2.3.2.3. Asynchronous Nature

The maximum number of asynchronous transactions that InDigoX will allow to be invoked over a given association is 3. The maximum number of asynchronous transactions that InDigoX will offer to invoke over a given association is 10 (though in reality will only be 1). Where a CStore SCU can take advantage of the asynchronous window, it has been shown to significantly increase storage throughput.

Table 4.2-15. Asynchronous nature of InDigoX.

Maximum number of asynchronous operations performed	3
Maximum number of asynchronous operations invoked	10

There is no limit to the number of outstanding Storage Commitment requests that can be received by InDigoX.

4.2.3.2.4. Implementation Identifying Information

InDigoX has the Implementation Class UID and Implementation Version Name specified in Table 4.2-16. The Implementation Version Name matches the version number of the InDigoX executable, which is currently 2.0.1. All versions of InDigoX in the 2.0.x.y family will adhere to this Conformance Statement.

Table 4.2-16 DICOM Implementation Class and Version for InDigoX AE.

Implementation Class UID	1.2.826.0.1.3867976.7.105
Implementation Version Name	2.0.x.y

4.2.3.3. Association Initiation Policy

4.2.3.3.1. Activity: Storage Commitment Notification over new Association

4.2.3.3.1.1. Description and Sequencing of Activities

A Storage Commitment request is deemed complete when all SOP Instances associated with it are either assigned an error condition or are robustly archived - the meaning of robustly archived is configurable by the Institution, but typically means that a SOP Instance is archived on two separate long-term storage nodes in the system, or the SOP Instance has been CStored to a 3rd party long-term DICOM Store such as a VNA, and a Storage Commitment request against that node has itself been successfully completed.

InDigoX will always negotiate a new Association in order to send Storage Commitment Push Model Notifications (N-EVENT-REPORT) for completed Storage Commitment requests. If there are multiple outstanding Notifications to be sent to the remote AE, InDigoX will attempt to send them over a single Association rather than requesting a new Association for each one. The Association will be released when all the N-EVENT-REPORTs for the peer AE have been sent. If the peer responds to the N-EVENT-REPORT with a status other than successful, or if an Association could not be initiated, the notification attempt will be retried every minute until it is successful.

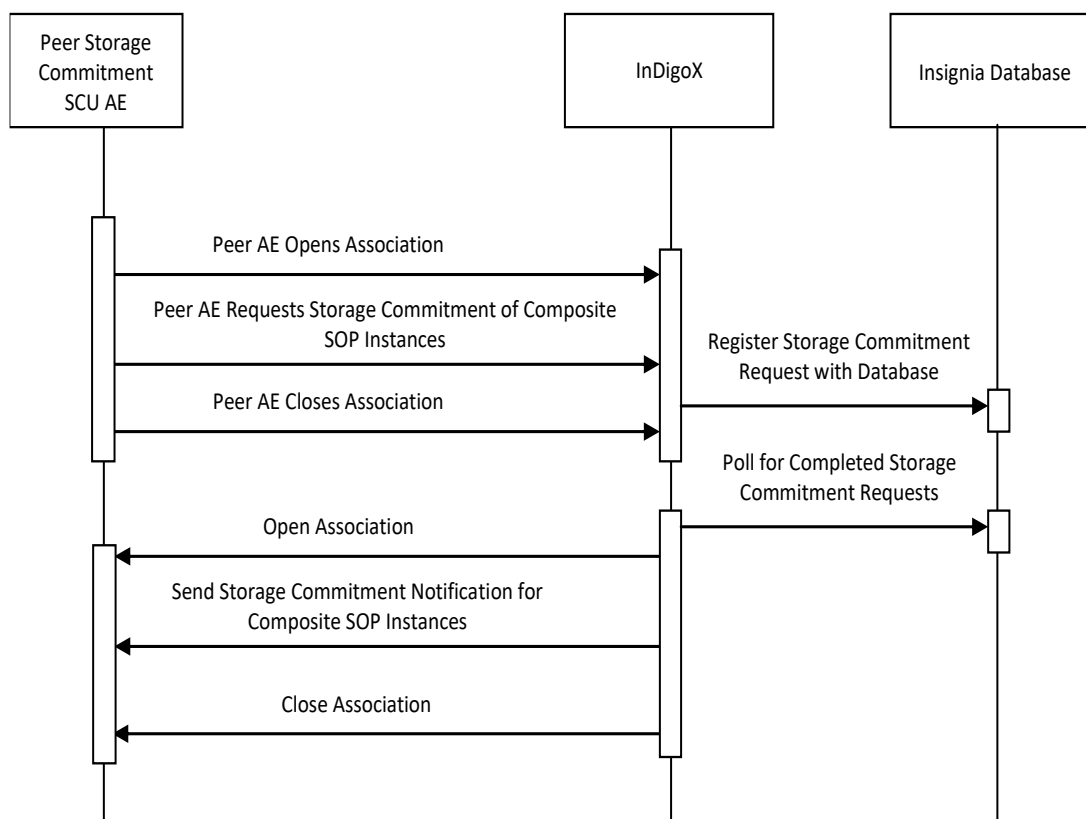


Figure 4.2-1. Sequencing of Activity: Send Commitment Notification over new Association.

4.2.3.3.1.2. Proposed Presentation Contexts

InDigoX will propose the following Presentation Context:

Table 4.2-17. Proposed Presentation Contexts by InDigoX.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.5.1.20.1	Implicit Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

4.2.3.3.1.3. SOP Specific Conformance for Storage Commitment SOP Class

InDigoX will not include the Media File-Set ID & UID attributes (0088,0130) and (0088,0140). The Retrieve AE Title attribute (0008,0054) will be set to the Inquire AE title associated with this Departmental Server.

Table 4.2-18 lists the possible Storage Commitment Failure Reasons (0008,1197) that may appear for SOP Instances in the N-EVENT-REPORT Failed SOP Sequence (0008,1198). In the case of the 'No Such Object Instance' failure occurring due to the object having been migrated from the Local Storage, a subsequent Storage Commitment request for the SOP Instance can be made to succeed by either causing the InSight System to internally route the SOP Instances to the Local storage, or the requesting AE can repeat the C-Store of the SOP Instance to InDigoX.

Table 4.2-18. Possible Values for InDigoX Storage Commitment N-EVENT-REPORT Failure Reason (0008,1197).

Failure Code	Reason
--------------	--------

0112 No Such Object Instance	The SOP Instance is not present on the Local Storage – there are three possible reasons for this: • it has not yet been received • InDigoX received the image, but the InSight Database refused to register the details due to data inconsistency • it has been migrated off the Local Storage node – this is unlikely to happen for at least 6 months after the C-Store event
0119 Class Instance Conflict	The SOP Instance is present, but does not have the SOP Class specified
0131 Duplicate Transaction UID	The Transaction UID already exists for an outstanding Storage Commitment Request

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**. In the event of errors causing an unexpected termination of an Association, Storage Commitment notifications will be retried every minute until a successful N-EVENT-REPORT response is received for the Transaction.

4.2.3.4. Association Acceptance Policy

4.2.3.4.1. Activity: Receipt of SOP Instances and Storage Commitment Requests

4.2.3.4.1.1. Description and sequencing of Activities

When InDigoX accepts an Association with a Presentation Context for a supported SOP Class, the remote Application Entity can send any number of CEcho, CStore or Storage Commitment Requests. When a Storage Commitment Request is received, the details are logged with the InSight Database. An N-EVENT-REPORT will be sent on a new association when completion is detected as described in section **4.2.3.3.1**. The remote Application Entity can release the Association at any point when no further commands are to be sent.

4.2.3.4.1.2. Accepted Presentation Contexts

Depending on the identity of the requesting AE, InDigoX will accept a subset of the Presentation Contexts for the Abstract Syntax / Transfer Syntax combinations listed in **Table 4.2-19**. Note, for clarity and to avoid unnecessary duplication of information, the Storage SOP Class Abstract Syntaxes from **Table 4.2-19** share one entry as they all support the same set of Transfer Syntaxes, Role and Extended Negotiation.

- The actual set of supported Abstract Syntaxes from the list in **Table 4.2-19** is configurable per remote AE, which allows certain SOP Classes to be supported for some remote AEs but not others.
- The set of supported Transfer Syntaxes is also configurable per remote AE. This can be used to eliminate known issues with some manufacturers' encodings of Undefined Length UN Sequences, and incorrect encoding of Lossless JPEG pixel data, for example.

Note that all Transfer Syntaxes are acceptable for the Verification SOP Class as there is no Information Object associated with the Service. Where multiple Transfer Syntaxes are offered in a Presentation Context for a supported Abstract Syntax, a Lossy Transfer Syntax will be accepted if and only if there is another Presentation Context for the Abstract Syntax with an acceptable Lossless Transfer Syntax, and a Lossy syntax has not yet been accepted for that Abstract Syntax. Otherwise the first supported Lossless or uncompressed Transfer Syntax will be selected for that Presentation Context, where 'first' is defined by the order in which the transfer syntaxes were listed by the Association Requestor for the Presentation Context.

Table 4.2-19. Accepted Presentation Contexts by InDigoX.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	Any		SCP	None
	1.2.840.10008.5.1.20.1	Implicit Little Endian	1.2.840.10008.1.2	SCP	None

Storage Commitment Push Model		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
The Storage SOP Classes in Table 4.2-13 See Table 4.2-13		Implicit Little Endian	1.2.840.10008.1.2	SCP	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
		JPEG Baseline (Process 1): Default Transfer Syntax for Lossy JPEG 8 Bit Image Compression	1.2.840.10008.1.2.4.50		
		JPEG Extended (Process 2 & 4): Default Transfer Syntax for Lossy JPEG 12 Bit Image Compression (Process 4 only)	1.2.840.10008.1.2.4.51		
		JPEG Lossless, Non-Hierarchical (Process 14)	1.2.840.10008.1.2.4.57		
		JPEG Lossless, Non-Hierarchical - First-Order Prediction (Process 14 [selection value 1])	1.2.840.10008.1.2.4.70		
		RLE Lossless	1.2.840.10008.1.2.5		

Note: Storage Service Extended Negotiation – if extended negotiation is requested, InDigoX will indicate that it is a Level 2 SCP, supports Signature Level 1, and may coerce Data Elements.

4.2.3.4.1.3. *SOP Specific Conformance for Verification SOP Class*

InDigoX provides standard conformance to the Verification SOP Class as an SCP.

4.2.3.4.1.4. *SOP Specific Conformance for Storage SOP Classes*

When InDigoX receives a Storage request, it will attempt to write the received SOP Instance to the Local Storage Node and register certain details of the object with the InSight System Database. Where pixel data exists in an object received in an uncompressed or lossless syntax, this is encapsulated on the local storage using the JPEG Lossless, Non-Hierarchical (Process 14) syntax. Where such an object is received in a Lossy transfer syntax, the object is written to the local storage preserving the existing lossy encapsulation.

InDigoX is a Level 2 (Full) conformant Storage SCP, so where the CStore succeeds, all Data Elements from the original object will be preserved, including Private and SOP Class Extended Elements. No special treatment is given to the Lossy Image Compression (0028,2110) attribute – it is preserved as received. Any Digital Signatures associated with the object are not preserved or replaced (Signature Level 1).

Once stored, if the images relate to a booking in the local Information System, the images are normally preserved on the InSight System or the associated VNA forever. Some deployments of the Disaster Recovery PACS may specify a maximum capacity of stored data and once this capacity is reached, objects are deleted in reverse time order to make space for newly acquired images. If images are received which do not relate to a booking in the local Information System, local PACS Policy dictates how long the images are retained on the system. All objects stored to an InDigoX instance can be retrieved from the InQUIRE component on any Departmental Server node in the system.

Coercion of data in the object will occur to update volatile demographics to the latest data received from the Institution Information System, however this coercion is performed by the InQUIRE CStore SCU when objects are retrieved from the system rather than when they are stored – see later section.

If a Duplicate SOP Instance for a non-rejected object is sent to InDigoX (as can happen if some objects in a multi-object series fail on the first send attempt and the whole series is subsequently resent), the new SOP will be ignored, and the CStore response status will either contain the status 0x0111: Duplicate SOP Instance, or, because that causes many modalities to terminate the association immediately and not send the rest of the Study, InDigoX can be configured to always return 0x0000: Success in this case.

Table 4.2-20. InDigoX CStore Response Status Reasons.

Service Status	Further Meaning	Error Code	Reasons
Success	Success	0000	The Composite SOP Instance has been successfully received, stored and registered with the InSight Database
Warning	Data Set does not match SOP Class	B007	If the SOP Class of the Data Set is different to the SOP Class in the Command Set, the object will be stored and registered, but this warning returned
Failure	Refused: Out of Resources	A700	Failed to write the object to local storage, probably because the local disk is full. Full details will be logged in the InDigoX error log. Error Comment (0000,0902) will read "Out of Resources"
	Cannot Understand	C000	Failed to register the object with the InSight Database. Full details will be logged in the InDigoX error log. Error Comment (0000,0902) will read "Failed to extract required data from object"
	Duplicate SOP Instance	0111	If configured to do so, InDigoX will return this status if a SOP Instance is received that already exists on the InSight System

If a communication failure occurs during the course of an Association, any objects that have been stored and registered with the InSight System are preserved, irrespective of whether the CStore Response has been successfully sent. If the communication failure occurs whilst part-way through receiving an object, that object will be discarded. The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination.**

4.2.3.4.1.5. *SOP Specific Conformance for Storage Commitment SOP Classes*

A remote AE can use the Storage Commitment service to request that it is notified when the InSight System has committed to the long-term ownership of a set of SOP Instances. A modality may use this information to determine when it is free to purge objects from its storage. The semantic of long-term ownership or robust archiving is configurable in the InSight System but is typically that the SOP Instance has been copied to two long-term storage nodes in the system, or that the SOP Instance has been CStored to a separate VNA, and a Storage Commitment has in turn been completed for the SOP Instance against the VNA. Once on long-term storage, the SOP Instances are available to the InSight System for the life of the system – this implies that where a Disaster Recovery PACS has been deployed with limited capacity, Storage Commitment will not be offered as a service.

SOP Instances for which Storage Commitment has been confirmed are always available for Query / Retrieve via any InQUIRE component on a Departmental Server node in the InSight System. Volatile demographic data will be updated when a SOP Instance is retrieved, see InQUIRE conformance in this document.

The Media File-Set ID and UID Attributes are not supported.

When InDigoX receives a Storage Commitment N-ACTION primitive, the Transaction UID and the set of referenced SOP Instance UIDs are registered with the InSight Database. InDigoX polls the database for completed transactions

once a minute and will open a new Association for the N-EVENT-REPORT notification when the Storage Commitment is complete, as described in section **4.2.3.3**

InDigoX will respond to the N-ACTION request with one of the following statuses:

Table 4.2-21. InDigoX Storage Commitment N-ACTION Response Statuses.

Status	Further Meaning	Error Code	Reason
Success	Success	0000	Transaction UID and Referenced SOP Instances registered with InSight System
Error	No Such Action Type	0123	Action Type was not 1
	Invalid Argument Value	0115	Required Attributes not present in the N-Action primitive. The Offending Element List data element (0000,0901) will be populated, as will Error Comment (0000,0902)
	Processing Failure	0110	The database call to register the Transaction UID and Referenced SOP Instances failed. Error Comment (0000,0902) will read "Failed to register Storage Commitment request"

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination.**

4.2.3.4.2. Activity: Receipt of IOCM KOS Object

4.2.3.4.2.1. Description and Sequencing of Activities

The InSight System can receive IOCM objects, where a sending system may wish to indicate that SOP Instances previously stored should be deprecated due to: Image Quality; Incorrect Parameters (eg view code, laterality etc); or Incorrect Procedure Step. The affected SOP Instances will be removed from the data hierarchy and no longer available for viewing or Query Retrieve. If any part of the affected study has already been sent to a separate long-term storage node, the IOCM Rejection Note KOS Document will be forwarded to that node.

4.2.3.4.2.2. Accepted Presentation Contexts

Table 4.2-22. Presentation Contexts Proposed by InQUIRE for IOCM KOS Object.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Implicit Little Endian	1.2.840.10008.1.2	SCP	None
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

4.2.3.4.2.3. SOP Specific Conformance for Storage of IOCM KOS Object

Any failure detected during the processing of a received IOCM KOS Object will be logged and flagged to system administrators.

4.2.4. InPort Application Entity Specification

4.2.4.1. SOP Classes

InPort provides Standard Conformance to the following DICOM V3.0 SOP Classes:

Table 4.2-23. SOP Classes for InPort AE.

SOP Class Name	SOP Class UID	SCU	SCP
Patient Root Query / Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.1.1	Yes	No
Patient Root Query / Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	Yes	No
Study Root Query / Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	Yes	No
Study Root Query / Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	Yes	No
Patient/Study Only Query/Retrieve Information Model–FIND	1.2.840.10008.5.1.4.1.2.3.1	Yes	No
Patient/Study Only Query/Retrieve Information Model–MOVE	1.2.840.10008.5.1.4.1.2.3.2	Yes	No

4.2.4.2. Association Policies

4.2.4.2.1. General

See **4.2.1 Common Application Entity Association Policies** for Application Context Name and Association Termination policies.

InPort only initiates Associations with remote AEs, it will not respond to incoming Association Requests.

4.2.4.2.2. Number of Associations

InPort will initiate one Association at a time over which it will perform a single CFind operation, and at the same time may have a configurable number of Associations (default is 5) open, performing a single CMove operation on each one. These Associations may be against the same or different remote AEs.

Table 4.2-24. Number of Simultaneous Associations as an Association Requester for InPort.

Maximum number of Simultaneous Associations	6 (1 CFind, Configurable number for CMove)
---	--

4.2.4.2.3. Asynchronous Nature

InPort will offer to invoke up to 10 asynchronous transactions on each Association, however in reality it will never invoke more than 1.

Table 4.2-25. Asynchronous nature as an Association Initiator for InPort.

Maximum number of outstanding asynchronous transactions invoked	10
---	----

4.2.4.2.4. Implementation Identifying Information

InPort has the Implementation Class UID and Implementation Version Name specified in Table 4.2-26. The Implementation Version Name matches the version number of the InPort executable, which is currently 2.0.1.0. All versions of InPort in the 2.0.x.y family will adhere to this Conformance Statement.

Table 4.2-26. DICOM Implementation Class and Version for InPort AE.

Implementation Class UID	1.2.826.0.1.3867976.7.107
Implementation Version Name	2.0.x.y

4.2.4.3. Association Initiation Policy

4.2.4.3.1. Activity: InSight System Interrogates Remote System

4.2.4.3.1.1. Description and Sequencing of Activities

The InSight System may need to interrogate a remote system for the information it holds regarding a certain Patient, Study or booking, or for all studies for a given time period. There are several scenarios where this is necessary, for example:

- Within an Institution, when the InSight Breast Screening PACS receives a booking for a Patient from the RIS / NBSS information feed, it may wish to interrogate an Institution's Radiology PACS for the details of any relevant studies in the Patient's imaging history
- Within an Institution, the Disaster Recovery PACS and VNA products are used for data duplication including migration/duplication of historic data, which may involve querying an Institution's PACS for details of studies taken on a certain date / date range
- Where multiple Institutions collaborate, the InSight PACS may wish to interrogate a collaborating PACS for details of a patient's history, either after receiving a booking for the patient or based on a User's request for information

Each CFind request will occur on a new Association, which will be released once the final response has been received. If no response has been received within 60 seconds, or the InPort service is shutdown while a CFind request is in progress, a C-FIND-CANCEL-RQ will be sent, and the Association will then be released once a non-pending CFind response (with status 'Cancelled' or otherwise) is received.

Depending on the information required by the InSight System the sequence of CFind requests will follow one of the following patterns:

4.2.4.3.1.2. Patient Demographic Query

A User wishes to find Patients that match a given Patient Name, Date of Birth, Sex combination.

- InPort opens a new Association
- A PATIENT Level (or STUDY Level if only the Study Root SOP Class was accepted) query is performed - the Patient Name field may contain wild cards.
- The Association is released
- The Matches are presented to the User, who will then probably select one patient on which to do a Patient History Query

4.2.4.3.1.3. Patient History Query

A User or the System wishes to retrieve details of the imaging history of a patient with a known Patient ID.

- InPort opens a new Association
- A STUDY Level query is performed, matching on the Patient ID
- The Association is released
- Then for each Study match:
 - InPort opens a new Association
 - A SERIES Level query is performed, matching on the Study Instance UID
 - The Association is released
 - The Study and Series results are reported to the System, which will present them to the User if required

4.2.4.3.1.4. Patient ID Query from Booking Reference

A User or the System wishes to retrieve details of the imaging history of the patient associated with a known booking reference, but the Patient ID is not known.

- InPort opens a new Study Root Association

- A STUDY Level query is performed, matching the booking on either Study ID or Accession number, depending on configuration
- The Patient ID is taken from the responses and reported to the System
- The Association is Released
- A Patient History Query is performed as above using the discovered Patient ID

4.2.4.3.1.5. Explicit Study Query

The System wishes to know the details of the Studies associated with a given booking or date range

- InPort opens a new Study Root Association
- A STUDY Level query is performed, matching on Study Date / Time range, or against the Booking Reference in the Study ID or Accession Number field, depending on configuration
- The Association is Released
- The matching studies are reported to the system

4.2.4.3.1.6. Proposed Presentation Contexts

InPort will propose Presentation Contexts from the following set (one Presentation Context per Abstract Syntax, each with multiple Transfer Syntaxes). InPort will only perform Hierarchical Queries, so Study Root is always proposed, Patient Root is proposed if Patient ID is known or a PATIENT Level query is requested, Patient / Study Only is proposed if the Level is PATIENT or the Level is STUDY and Patient ID is known.

Table 4.2-27. Presentation Contexts proposed by InPort for Remote AE Query.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Patient Root Q/R Information Model – FIND	1.2.840.10008.5.1.4.1.2.1.1	Implicit Little Endian	1.2.840.10008.1.2	SCU	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
Study Root Q/R Information Model – FIND	1.2.840.10008.5.1.4.1.2.2.1	Implicit Little Endian	1.2.840.10008.1.2	SCU	
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
Patient / Study Only Q/R Information Model – FIND	1.2.840.10008.5.1.4.1.2.3.1	Implicit Little Endian	1.2.840.10008.1.2	SCU	
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

Note: Extended Negotiation – InPort does not request Relational Queries or combined Date-Time matching, but will request Fuzzy Semantic person name matching for the Patient Demographic Query if requested to do so by the User.

When a CFind command is then issued on the Association, the most appropriate Presentation Context accepted from those offered will be used. For the scenarios outlined above, the Abstract Syntax orders of preference are as follows:

Table 4.2-28. Order of Preference for Presentation Contexts Usage for InPort Remote AE Query.

Scenario	Abstract Syntax Order of Preference		
Patient Demographic Query	Patient Root	Patient / Study Only	Study Root
Patient History Query • Associated Series Level Query	Study Root Study Root	Patient Root Patient Root	Patient / Study Only -
Patient ID Query from Booking Reference	Study Root	-	-
Explicit Study Query	Study Root	-	-

4.2.4.3.2. SOP Specific Conformance for Patient Root and Patient/Study Only CFind

InPort may perform Patient Root and Patient / Study Only queries at the PATIENT or STUDY level. For the Patient Root SOP Class it may also perform SERIES level queries. IMAGE level queries will not be performed.

Neither Relational Queries nor combined date and time matching will be requested. The user may request that the Patient Name in a Patient Demographic Query be matched using Fuzzy Semantic, in which case InPort will attempt to negotiate Fuzzy Semantic Person Name matching.

Specific Character Set (0008,0005) will only be present if the Patient Name in a Patient Demographic Query contains characters outside the default repertoire. If present the character set will be ISO Latin 1 (ISO_IR 100). If the Specific Character Set attribute (0008,0005) is present in the Result Data Set and set to Unicode UTF-8 (ISO_IR 192), strings will be converted to ISO Latin 1 if possible. In all other cases the Character Set is ignored and strings are assumed to be ISO Latin 1. Timezone Offset from UTC is not included in the query and will be ignored if present in a response. The following tables specify the contents of the Request Identifiers for each Query Level:

Table 4.2-29. InPort Patient Root & Patient / Study Only PATIENT Level Request Identifier.

Name	Tag	Matching Type
Patient Name	(0010,0010)	Single Value, Wild Card, Universal
Patient ID	(0010,0020)	Single Value, Universal
Patient ID Issuer	(0010,0021)	Universal
Patient ID Type	(0010,0022)	Universal
Patient ID Issuer Qualifier SQ	(0010,0024)	Universal Sequence
Other Patient ID SQ	(0010,1002)	Universal Sequence, Sequence
> Patient ID	(0010,0020)	Single Value, Universal
> Patient ID Issuer	(0010,0021)	Universal
> Type of Patient ID	(0010,0022)	Universal
> Patient ID Issuer Qualifier SQ	(0010,0024)	Universal Sequence
Patient Date of Birth	(0010,0030)	Single Value, Universal
Patient Sex	(0010,0040)	Single Value, Universal
Other Patient IDs	(0010,1000)	Universal
Number of Patient Related Studies	(0020,1200)	Universal
Number of Patient Related Series	(0020,1202)	Universal
Number of Patient Related Instances	(0020,1204)	Universal

Note: if the Patient ID is provided for Single Value matching, all other fields will be specified for Universal Matching

Table 4.2-30. InPort Patient Root & Patient / Study Only STUDY Level Request Identifier.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value
Study Instance UID	(0020,000D)	Universal
Study Date	(0008,0020)	Universal
Study Time	(0008,0030)	Universal
Accession Number	(0008,0050)	Universal
Modalities In Study	(0008,0061)	Universal
Study ID	(0020,0010)	Universal
Study Description	(0020,1030)	Universal
Referring Physician	(0008,0090)	Universal
Procedure Code Sequence	(0008,1032)	Universal Sequence
Name of Physician(s) Reading Study	(0008,1060)	Universal
Reason For Performed Procedure SQ	(0040,1032)	Universal Sequence
Number of Study Related Series	(0020,1206)	Universal
Number of Study Related Instances	(0020,1208)	Universal

Table 4.2-31. InPort Patient Root SERIES Level Request Identifier.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value
Study Instance UID	(0020,000D)	Single Value
Modality	(0008,0060)	Universal
Series Instance UID	(0020,000E)	Universal
Series Number	(0020,0011)	Universal
Series Description	(0008,103E)	Universal
Series Date	(0008,0021)	Universal
Series Time	(0008,0031)	Universal
Body Part Examined	(0018,0015)	Universal
Performing Physician	(0008,1050)	Universal
Patient Position	(0018,5100)	Universal
Frame Of Reference	(0020,0052)	Universal
Laterality	(0020,0060)	Universal
Device Model	(0008,1090)	Universal
Manufacturer	(0008,0070)	Universal
Request Attribute Sequence	(0040,0275)	Universal Sequence
Number of Series Related Instances	(0020,1209)	Universal

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination** an error occurs during a CFind command, no results will be presented to the InSight Database. The InSight System may queue the CFind request to be retried if it was generated by a system rule rather than User interaction.

4.2.4.3.3. SOP Specific Conformance for Study Root CFind

InPort may perform Study Root queries at the STUDY or SERIES level. IMAGE level queries will not be performed. Neither Relational Queries nor combined date and time matching will be requested. The user may request that the Patient Name in a Patient Demographic Query be matched using Fuzzy Semantic, in which case InPort will attempt to negotiate Fuzzy Semantic Person Name matching. If a Presentation Context for the Patient Root or Patient / Study Only SOP Class has been accepted, they will be used in preference of the Study Root SOP Class for the Patient Demographic Query, for the other InPort Query use cases, Study Root CFind is the preferred Abstract Syntax.

Specific Character Set (0008,0005) will only be present if the Patient Name in a Patient Demographic Query contains characters outside the default repertoire. If present the character set will be ISO Latin 1 (ISO_IR 100). If the Specific Character Set (0008,0005) is present in the Result Data Set and set to Unicode UTF-8 (ISO_IR 192), strings will be converted to ISO Latin 1 if possible. In all other cases the Character Set is ignored, and strings are assumed to be ISO Latin 1. Time zone Offset from UTC is not included in the query and will be ignored if present in a response. The following tables specify the contents of the Request Identifiers for each Query Level:

Table 4.2-32. InPort Study Root STUDY Level Request Identifier.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value, Universal
Patient Name	(0010,0010)	Single Value, Wild Card, Universal
Patient ID Issuer	(0010,0021)	Universal
Patient ID Type	(0010,0022)	Universal
Patient ID Issuer Qualifier SQ	(0010,0024)	Universal Sequence
Other Patient ID SQ	(0010,1002)	Universal Sequence, Sequence
> Patient ID	(0010,0020)	Single Value, Universal
> Patient ID Issuer	(0010,0021)	Universal

> Type of Patient ID	(0010,0022)	Universal
> Patient ID Issuer Qualifier SQ	(0010,0024)	Universal Sequence
Patient Date of Birth	(0010,0030)	Single Value, Universal
Patient Sex	(0010,0040)	Single Value, Universal
Other Patient IDs	(0010,1000)	Universal
Study Instance UID	(0020,000D)	Universal
Study Date	(0008,0020)	Single Value, Range or Universal
Study Time	(0008,0030)	Range or Universal
Accession Number	(0008,0050)	Single Value or Universal
Modalities In Study	(0008,0061)	Universal
Study ID	(0020,0010)	Single Value or Universal
Study Description	(0020,1030)	Universal
Referring Physician	(0008,0090)	Universal
Procedure Code Sequence	(0008,1032)	Universal Sequence
Name of Physician(s) Reading Study	(0008,1060)	Universal
Reason For Performed Procedure SQ	(0040,1032)	Universal Sequence
Number of Study Related Series	(0020,1206)	Universal
Number of Related Instances	(0020,1208)	Universal

Note: 1) If one of Patient ID, Accession Number or Study ID is provided for Single Value Matching, all other fields will be specified for Universal Matching.

2) If Study Date is provided for Range Matching, all other fields will be specified for Universal Matching.

3) If Study Date is provided for Single Value matching, Study Time will be specified for either Range matching or Universal Matching, all other fields will be specified for Universal Matching.

Table 4.2-33. InPort Study Root SERIES Level Request Identifier.

Name	Tag	Matching Type
Study Instance UID	(0020,000D)	Single Value
Modality	(0008,0060)	Universal
Series Instance UID	(0020,000E)	Universal
Series Number	(0020,0011)	Universal
Series Description	(0008,103E)	Universal
Series Date	(0008,0021)	Universal
Series Time	(0008,0031)	Universal
Body Part Examined	(0018,0015)	Universal
Performing Physician	(0008,1050)	Universal
Patient Position	(0018,5100)	Universal
Frame Of Reference	(0020,0052)	Universal
Laterality	(0020,0060)	Universal
Device Model	(0008,1090)	Universal
Manufacturer	(0008,0070)	Universal
Request Attribute Sequence	(0040,0275)	Universal Sequence
Number of Series Related Instances	(0020,1209)	Universal

4.2.4.3.4. Response Status Handling

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**, handling of CFind SOP Class specific result statuses are handled as described in **Table 4.2-34**. If an error occurs during a CFind command, no results will be presented to the InSight Database. The InSight System may automatically queue the CFind request to be retried after a period if it was generated by a system rule rather than User interaction.

Table 4.2-34. InPort Response Statuses for Query Remote AE Request.

Status	Further Meaning	Error Code	Behaviour
--------	-----------------	------------	-----------

Refused	Out of Resources	A700	Current Query is terminated, accumulated results are discarded and Error Comment (0000,0902) is logged; remaining queries continue
Error	Identifier does not match SOP Class	A900	
	Unable to Process	Cxxx	
Cancel	Matching terminated due to Cancel Request	FE00	Expected if Cancel Request issued. Current Query is terminated, and accumulated results are discarded; remaining queries continue
Success	Matching is complete – No final Identifier is supplied	0000	Accumulated results from Query are reported to the InSight system
Pending	Matches are continuing - Current Match is supplied and any Optional Keys were supported in the same manner as Required Keys	FF00	This result is added to the accumulating set of results for the query
	Matches are continuing - Warning that one or more Optional Keys were not supported for existence and/or matching for this Identifier	FF01	

4.2.4.3.5. Activity: InSight System Requires Objects Residing on Remote System

4.2.4.3.5.1. Description and Sequencing of Activities

Once the Study Instance UIDs of the Studies contained on a Remote System for a given Patient, Booking or Study Date/ Time Range have been established (by InPort interrogation, or by other means), InPort will issue STUDY Level CMove requests for those Studies that the InSight System calculates that it requires, or a User requests. Each CMove request will be issued on a new Association; the Association will be released when the Final Response is received. The CMove Destination will be set to the AE Title of the InDigoX Instance residing on the Departmental Server node.

InPort will send a C-MOVE-CANCEL-RQ for an active CMove if the User cancels a User initiated CMove request, or if InPort is shutdown while CMove requests are in progress. The Association will then be released when a non-pending CMove response is received (with status 'Cancelled' or otherwise).

4.2.4.3.5.2. Proposed Presentation Contexts

InPort will propose the following Presentation Contexts for the STUDY Level CMove request.

Table 4.2-35. Presentation Contexts proposed by InPort for Remote AE Retrieve.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Patient Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Implicit Little Endian	1.2.840.10008.1.2	SCU	See Note
Patient Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit Little Endian	1.2.840.10008.1.2.1	SCU	
Patient Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.1.2	Explicit Big Endian	1.2.840.10008.1.2.2	SCU	
Study Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Implicit Little Endian	1.2.840.10008.1.2	SCU	

Study Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit Little Endian	1.2.840.10008.1.2.1	SCU	
Study Root Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.2.2	Explicit Big Endian	1.2.840.10008.1.2.2	SCU	
Patient / Study Only Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Implicit Little Endian	1.2.840.10008.1.2	SCU	
Patient / Study Only Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Explicit Little Endian	1.2.840.10008.1.2.1	SCU	
Patient / Study Only Q/R Information Model – MOVE	1.2.840.10008.5.1.4.1.2.3.2	Explicit Big Endian	1.2.840.10008.1.2.2	SCU	

Note: InPort will attempt to negotiate Relational Retrieval

The three Abstract Syntaxes will always be offered with Relational Retrieval extended negotiation, as this means a STUDY Level retrieval for a known Study Instance UID can be performed even if the Patient ID is not known.

If Patient ID and Study Instance UID are known, the order of preference for the Presentation Context to use for the CMove request will be Patient Root - Study Root - Patient/Study Only.

If only Study Instance UID is known, the order of preference for the Presentation Context used will be Study Root - Patient Root - Patient/Study Only. Patient Root and Patient/Study Only will only be used if the peer has accepted those Abstract Syntaxes with Relational Retrieval.

4.2.4.3.5.3. SOP Specific Conformance for Retrieve Service Classes

InPort will only invoke STUDY Level CMove requests, each of which will contain a single Study Instance UID (0020,000D). It will attempt to negotiate Relational Retrieval. If the Patient Root or Patient/Study Only SOP Class was chosen and Relational Retrieval was not negotiated, Patient Id (0010,0020) will also be present in the retrieve request. This will be the Patient Id received from the remote system in the CFind result for the Study. The CMove Destination for all Retrieval Requests will be set to the AE Title of the InDigoX instance on the Departmental Server node.

4.2.4.3.5.4. Response Status Handling

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**, handling of CMove SOP Class specific result statuses are handled as described in **Table 4.2-36**. In the event of an unexplained failure of the CMove command, the InSight System will queue the CMove request to be retried.

Table 4.2-36. InPort Response Statuses for Move Study Request.

Status	Further Meaning	Error Code	Behaviour
Refused	Out of Resources - Unable to calculate number of matches	A701	Retrieval is terminated, Error Comment (0000,0902) is logged if present. Number of sub-operations Remaining, Complete, Failed and Warning - (0000,1020), (0000,1021), (0000,1022), (0000,1023) respectively - are reported to the InSight System, if present
Refused	Out of Resources – Unable to perform sub-operations	A702	
Refused	Move Destination Unknown	A801	
Failed	Identifier does not match SOP Class	A900	
Failed	Unable to Process	Cxxx	

Cancel	Matching terminated due to Cancel Request	FE00	Expected if Cancel Request issued. Retrieval is terminated, Number of sub-operations Remaining, Complete, Failed and Warning - (0000,1020), (0000,1021), (0000,1022), (0000,1023) respectively - are reported to the InSight System
Warning	Sub-operations Complete- One or more Failures	B000	Retrieval is complete- Number of sub-operations Complete, Failed and Warning - (0000,1021), (0000,1022), (0000,1023) respectively - are reported to the InSight System
Success	Sub-operations complete – No failures	0000	Retrieval is complete- Number of sub-operations Complete, Failed and Warning - (0000,1021), (0000,1022), (0000,1023) respectively - are reported to the InSight System
Pending	Sub-operations continuing	FF00	Progress is logged with the InSight system if the previous logged Pending result was received over 1 second ago. The number of sub-operations Remaining, Complete, Failed and Warning - (0000,1020), (0000,1021), (0000,1022), (0000,1023) respectively – are reported to the system.

4.2.4.3.5.5. Sub-Operation Dependent Behaviour

InPort is unaware of the activities which are taking place between the remote system and the InDigoX instance nominated as the Destination in the CMove request. Once the C-MOVE has been initiated it runs to completion (or failure), and InPort is only aware of progress and completion as described in the C-MOVE response command message(s). There is no attempt by InPort to confirm that instances have actually been successfully received or locally stored, this is dealt with by the InSight System at a higher level.

Whether or not the remote AE attempts to retry any failed C-STORE sub-operations is beyond the control of InPort. If the association on which the C-MOVE was issued is aborted for any reason, the continuation of the C-STORE sub-operations is entirely dependent on the remote AE; the InDigoX instance will continue to accept associations and storage operations regardless.

4.2.4.4. Association Acceptance Policy

InPort does not accept Associations.

4.2.5. Inquire Application Entity Specification

4.2.5.1. SOP Classes

Inquire provides Standard Conformance to the following DICOM V3.0 SOP Classes:

Table 4.2-37. SOP Classes for Inquire AE.

SOP Class Name	SOP Class UID	SCU	SCP
Verification	1.2.840.10008.1.1	No	Yes
Storage Commitment Push Model	1.2.840.10008.1.20.1	Yes	No
Computed Radiography Image Storage	1.2.840.10008.5.1.4.1.1.1	Yes	No
Digital X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.1	Yes	No
Digital X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.1.1	Yes	No
Digital Mammography XRay Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.2	Yes	No
Digital Mammography XRay Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.2.1	Yes	No

Digital Intra-oral X-Ray Image Storage – For Presentation	1.2.840.10008.5.1.4.1.1.1.3	Yes	No
Digital Intra-oral X-Ray Image Storage – For Processing	1.2.840.10008.5.1.4.1.1.1.3.1	Yes	No
CT Image Storage	1.2.840.10008.5.1.4.1.1.2	Yes	No
Ultrasound Multi-frame Image Storage	1.2.840.10008.5.1.4.1.1.3.1	Yes	No
MR Image Storage	1.2.840.10008.5.1.4.1.1.4	Yes	No
MR Spectroscopy Storage	1.2.840.10008.5.1.4.1.1.4.2	Yes	No
Ultrasound Image Storage	1.2.840.10008.5.1.4.1.1.6.1	Yes	No
Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7	Yes	No
Multi-frame Single Bit Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.1	Yes	No
Multi-frame Greyscale Byte Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.2	Yes	No
Multi-frame Greyscale Word Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.3	Yes	No
Multi-frame True Colour Secondary Capture Image Storage	1.2.840.10008.5.1.4.1.1.7.4	Yes	No
12-lead ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.1	Yes	No
General ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.2	Yes	No
Ambulatory ECG Waveform Storage	1.2.840.10008.5.1.4.1.1.9.1.3	Yes	No
Hemodynamic Waveform Storage	1.2.840.10008.5.1.4.1.1.9.2.1	Yes	No
Cardiac Electrophysiology Waveform Storage	1.2.840.10008.5.1.4.1.1.9.3.1	Yes	No
Basic Voice Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.1	Yes	No
General Audio Waveform Storage	1.2.840.10008.5.1.4.1.1.9.4.2	Yes	No
Arterial Pulse Waveform Storage	1.2.840.10008.5.1.4.1.1.9.5.1	Yes	No
Respiratory Waveform Storage	1.2.840.10008.5.1.4.1.1.9.6.1	Yes	No
Greyscale Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.1	Yes	No
Colour Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.2	Yes	No
Pseudo-Colour Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.3	Yes	No
Blending Softcopy Presentation State Storage	1.2.840.10008.5.1.4.1.1.11.4	Yes	No
X-Ray Angiographic Image Storage	1.2.840.10008.5.1.4.1.1.12.1	Yes	No
X-Ray Radiofluoroscopic Image Storage	1.2.840.10008.5.1.4.1.1.12.2	Yes	No
Breast Tomosynthesis Image Storage	1.2.840.10008.5.1.4.1.1.13.1.3	Yes	No
Breast Projection X-Ray Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.13.1.4	Yes	No
Breast Projection X-Ray Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.13.1.5	Yes	No
Intravascular Optical Coherence Tomography Image Storage - For Presentation	1.2.840.10008.5.1.4.1.1.14.1	Yes	No
Intravascular Optical Coherence Tomography Image Storage - For Processing	1.2.840.10008.5.1.4.1.1.14.2	Yes	No
Nuclear Medicine Image Storage	1.2.840.10008.5.1.4.1.1.20	Yes	No
Raw Data Storage	1.2.840.10008.5.1.4.1.1.66	Yes	No
Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.1	Yes	No
Spatial Fiducials Storage	1.2.840.10008.5.1.4.1.1.66.2	Yes	No
Deformable Spatial Registration Storage	1.2.840.10008.5.1.4.1.1.66.3	Yes	No
Surface Segmentation Storage	1.2.840.10008.5.1.4.1.1.66.5	Yes	No
Tractography Results Storage	1.2.840.10008.5.1.4.1.1.66.6	Yes	No
Real World Value Mapping Storage	1.2.840.10008.5.1.4.1.1.67	Yes	No
Surface Scan Mesh Storage	1.2.840.10008.5.1.4.1.1.68.1	Yes	No
Surface Scan Point Cloud Storage	1.2.840.10008.5.1.4.1.1.68.2	Yes	No
VL Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1	Yes	No
Video Endoscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.1.1	Yes	No
VL Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2	Yes	No
Video Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.2.1	Yes	No
VL Slide-Coordinates Microscopic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.3	Yes	No
VL Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4	Yes	No
Video Photographic Image Storage	1.2.840.10008.5.1.4.1.1.77.1.4.1	Yes	No
Ophthalmic Photography 8 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.1	Yes	No
Ophthalmic Photography 16 Bit Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.2	Yes	No

Stereometric Relationship Storage	1.2.840.10008.5.1.4.1.1.77.1.5.3	Yes	No
Ophthalmic Tomography Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.4	Yes	No
Wide Field Ophthalmic Photography Stereographic Projection Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.5	Yes	No
Wide Field Ophthalmic Photography 3D Coordinates Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.6	Yes	No
Ophthalmic Optical Coherence Tomography En Face Image Storage	1.2.840.10008.5.1.4.1.1.77.1.5.7	Yes	No
Ophthalmic Optical Coherence Tomography B-scan Volume Analysis Storage	1.2.840.10008.5.1.4.1.1.77.1.5.8	Yes	No
VL Whole Slide Microscopy Image Storage	1.2.840.10008.5.1.4.1.1.77.1.6	Yes	No
Lensometry Measurements Storage	1.2.840.10008.5.1.4.1.1.78.1	Yes	No
Autorefraction Measurements Storage	1.2.840.10008.5.1.4.1.1.78.2	Yes	No
Keratometry Measurements Storage	1.2.840.10008.5.1.4.1.1.78.3	Yes	No
Subjective Refraction Measurements Storage	1.2.840.10008.5.1.4.1.1.78.4	Yes	No
Visual Acuity Measurements Storage	1.2.840.10008.5.1.4.1.1.78.5	Yes	No
Spectacle Prescription Report Storage	1.2.840.10008.5.1.4.1.1.78.6	Yes	No
Ophthalmic Axial Measurements Storage	1.2.840.10008.5.1.4.1.1.78.7	Yes	No
Intraocular Lens Calculations Storage	1.2.840.10008.5.1.4.1.1.78.8	Yes	No
Macular Grid Thickness and Volume Report Storage	1.2.840.10008.5.1.4.1.1.79.1	Yes	No
Ophthalmic Visual Field Static Perimetry Measurements Storage	1.2.840.10008.5.1.4.1.1.80.1	Yes	No
Ophthalmic Thickness Map Storage	1.2.840.10008.5.1.4.1.1.81.1	Yes	No
Corneal Topography Map Storage	1.2.840.10008.5.1.4.1.1.82.1	Yes	No
Basic Text SR	1.2.840.10008.5.1.4.1.1.88.11	Yes	No
Enhanced SR	1.2.840.10008.5.1.4.1.1.88.22	Yes	No
Comprehensive SR	1.2.840.10008.5.1.4.1.1.88.33	Yes	No
Comprehensive 3d SR Storage	1.2.840.10008.5.1.4.1.1.88.34	Yes	No
Extensible SR Storage	1.2.840.10008.5.1.4.1.1.88.35	Yes	No
Procedure Log Storage	1.2.840.10008.5.1.4.1.1.88.40	Yes	No
Mammography CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.50	Yes	No
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Yes	No
Chest CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.65	Yes	No
X-Ray Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.67	Yes	No
Radiopharmaceutical Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.68	Yes	No
Colon CAD SR Storage	1.2.840.10008.5.1.4.1.1.88.69	Yes	No
Implantation Plan SR Storage	1.2.840.10008.5.1.4.1.1.88.70	Yes	No
Acquisition Context SR Storage	1.2.840.10008.5.1.4.1.1.88.71	Yes	No
Simplified Adult Echo SR Storage	1.2.840.10008.5.1.4.1.1.88.72	Yes	No
Patient Radiation Dose SR Storage	1.2.840.10008.5.1.4.1.1.88.73	Yes	No
Planned Imaging Agent Administration SR Storage	1.2.840.10008.5.1.4.1.1.88.74	Yes	No
Performed Imaging Agent Administration SR Storage	1.2.840.10008.5.1.4.1.1.88.75	Yes	No
Content Assessment Results Storage	1.2.840.10008.5.1.4.1.1.90.1	Yes	No
Encapsulated PDF Storage	1.2.840.10008.5.1.4.1.1.104.1	Yes	No
Encapsulated CDA Storage	1.2.840.10008.5.1.4.1.1.104.2	Yes	No
Encapsulated STL Storage	1.2.840.10008.5.1.4.1.1.104.3	Yes	No
Positron Emission Tomography Image Storage	1.2.840.10008.5.1.4.1.1.128	Yes	No
RT Image Storage	1.2.840.10008.5.1.4.1.1.481.1	Yes	No
RT Dose Storage	1.2.840.10008.5.1.4.1.1.481.2	Yes	No
RT Structure Set Storage	1.2.840.10008.5.1.4.1.1.481.3	Yes	No
RT Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.4	Yes	No
RT Plan Storage	1.2.840.10008.5.1.4.1.1.481.5	Yes	No
RT Brachy Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.6	Yes	No
RT Treatment Summary Record Storage	1.2.840.10008.5.1.4.1.1.481.7	Yes	No
RT Ion Plan Storage	1.2.840.10008.5.1.4.1.1.481.8	Yes	No
RT Ion Beams Treatment Record Storage	1.2.840.10008.5.1.4.1.1.481.9	Yes	No

RT Physician Intent Storage	1.2.840.10008.5.1.4.1.1.481.10	Yes	No
RT Segment Annotation Storage	1.2.840.10008.5.1.4.1.1.481.11	Yes	No
RT Radiation Set Storage	1.2.840.10008.5.1.4.1.1.481.12	Yes	No
C-Arm Photon-Electron Radiation Storage	1.2.840.10008.5.1.4.1.1.481.13	Yes	No
Patient Root Query / Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.1.2	No	Yes
Study Root Query / Retrieve Information Model - FIND	1.2.840.10008.5.1.4.1.2.2.1	No	Yes
Study Root Query / Retrieve Information Model - MOVE	1.2.840.10008.5.1.4.1.2.2.2	No	Yes
Patient/Study Only Query/Retrieve Information Model – FIND (Retired)	1.2.840.10008.5.1.4.1.2.3.1	No	Yes
Patient/Study Only Query/Retrieve Information Model – MOVE (Retired)	1.2.840.10008.5.1.4.1.2.3.2	No	Yes

InQure will send Composite Objects using the Storage SOP Class that was used when the Object was received by InDigoX.

4.2.5.2. Association Policies

4.2.5.2.1. General

See 4.2.1 Common Application Entity Association Policies for Application Context Name and Association Rejection and Termination policies.

InQure can both initiate Associations and listen for Association Requests from Remote AEs. It will accept Associations for Verification and the Composite Object Query / Retrieve Service Classes. It will propose Associations for the Storage Service Classes and the Storage Commitment (Push Model) Service Class.

4.2.5.2.2. Number of Associations

The maximum number of simultaneous associations that InQure will accept is configurable, and defaults to 5. There is no restriction within this limit for the maximum number of simultaneous associations acceptable from any given remote Application Entity.

InQure will initiate a Storage Association for each open CMove request, and in addition may initiate a configurable number (default 10) of simultaneous Storage Associations to route objects to remote AEs due to rules in the InSight System. Within this limit, InQure does not restrict the number of simultaneous Associations which may be open to a particular Remote AE at any given time.

Table 4.2-38. Number of Simultaneous Associations for InQure.

Maximum number of simultaneous requested Associations	5 (Configurable)
Maximum number of simultaneous proposed Associations	15 (Configurable)

4.2.5.2.3. Asynchronous Nature

The maximum number of asynchronous transactions that InQure will allow to be invoked over a given association is 3. The maximum number of asynchronous transactions that InQure will offer to invoke over a given association is 10. If agreed in the negotiation, the Storage Services will make use of the Asynchronous window when sending Objects, as it has been shown to increase throughput.

Table 4.2-39. Asynchronous nature of InQure.

Maximum number of asynchronous operations performed	3
Maximum number of asynchronous operations invoked	10

4.2.5.2.4. Implementation Identifying Information

InQure has the Implementation Class UID and Implementation Version Name specified in **Table 4.2-40**. The Implementation Version Name matches the version number of the InQure executable, which is currently 2.0.1. All versions of InQure in the 2.0.x.y family will adhere to this Conformance Statement.

Table 4.2-40. DICOM Implementation Class and Version for InQure AE.

Implementation Class UID	1.2.826.0.1.3867976.7.100
Implementation Version Name	2.0.x.y

4.2.5.3. Association Initiation Policy

4.2.5.3.1. Activity: Storage of Composite Objects to Remote AE

4.2.5.3.1.1. Description and Sequencing of Activities

InQure will initiate a new Association in response to it receiving a CMove request from a Remote AE, or when triggered to route objects to a Remote AE by rules in the InSight System. It will attempt to send all required objects for the CMove request or the routing event, then release the Association.

4.2.5.3.1.2. Proposed Presentation Contexts

InQure will only propose Presentation Contexts for the set of SOP Classes represented in the set of objects to send to the Remote AE. The set of proposed Transfer Syntaxes is configurable per Remote AE from the set in **Table 4.2-41**, which allows InQure to avoid known problems with some manufacturers' incorrect implementations of Undefined Length Unknown Sequences, JPEG encoding, etc.

For each required Abstract Syntax, one Presentation Context will be offered with all peer-supported Transfer Syntaxes and, if the object contains Pixel Data, one Presentation Context will be offered with just the Transfer Syntax that represents the storage of the object on the InSight System (currently this is Lossless JPEG, Non-Hierarchical unless the object was originally received in a lossy syntax, in which case the original lossy syntax is preserved and will be offered) – this is the preferred Transfer Syntax as no encapsulation conversion will be required, and this Presentation Context will be used if accepted. Note – Lossy syntaxes will not be offered unless objects of that SOP Class are held in a lossy format on storage. InQure will never use a lossy syntax for an object held on storage in a lossless format. **Table 4.2-41**, shows the Transfer Syntaxes that may be offered.

Table 4.2-41. Presentation Contexts Proposed by InQure.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage SOP Classes where the Composite Object does not contain the Pixel Data Element	See Table 3.8-37	Implicit Little Endian	1.2.840.10008.1.2	SCU	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
Storage SOP Classes where the Composite Object	See Table 3.8-37	Implicit Little Endian	1.2.840.10008.1.2	SCU	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

contains the Pixel Data Element (ie Image Classes) in Table 3.8-37	JPEG Baseline (Process 1): Default Transfer Syntax for Lossy JPEG 8 Bit Image Compression	1.2.840.10008.1.2.4.5 0		
	JPEG Extended (Process 2 & 4): Default Transfer Syntax for Lossy JPEG 12 Bit Image Compression (Process 4 only)	1.2.840.10008.1.2.4.5 1		
	JPEG Lossless, Non-Hierarchical (Process 14)	1.2.840.10008.1.2.4.5 7		
	JPEG Lossless, Non-Hierarchical - First-Order Prediction (Process 14 [selection value 1])	1.2.840.10008.1.2.4.7 0		

Note: Storage Service Extended Negotiation – Inquire includes the extended negotiation item in the Association Request to allow the SCP to indicate its level of support.

4.2.5.3.1.3. *SOP Specific Conformance for Storage Service Classes*

Inquire sends SOP Instances that have originally been received by the InSight System via InDigoX. InDigoX is a type 2 Storage SCP, so all Optional and Private Data Elements and Functional Groups are preserved; as such, the exact set of Data Elements present in instances of each SOP Class will be detailed in the Conformance Statements of the systems that originally sent the SOP Instances to InDigoX, and cannot be defined here.

Inquire does not support Referenced Pixel Data Transfer Syntaxes.

If an image is held in a Lossless format, the Lossy transfer syntaxes will not be offered – there is no conversion from Lossless to Lossy compression. If an image is held in a Lossy Format, only the appropriate lossy transfer syntax will be offered. There is no translation from Lossy to Lossless; if the Presentation Context offering the Lossy Transfer Syntax for the Abstract Syntax is not accepted, then no attempt will be made to CStore the Lossy images.

The status contained in a CStore response will be reported to either the CMove originator as part of the pending and final responses, or the InSight System if the CStores are in response to a Routing event - be it Successful, Warning or a Failure. In the event of an individual CStore command failing, a CStore attempt will still be made for all other SOP Instances in the CMove request or InSight Routing set. The failed command will not automatically be retried but a detailed error will be written to the Inquire error log.

Inquire will not attempt to update SOP Instances from retired SOP Classes to the new SOP Classes, and it will not fall back to using a related General SOP Class if a Specialised SOP Class is rejected.

When sending images, certain Volatile Patient Demographic information will be updated to match the latest information from the Institution's information System, or where errors of hierarchy have been corrected by the InSight System tools. Optional Fields for a given IOD will only be updated if they are already present in the SOP Instance, not added. The fields that may be updated are as follows:

Table 4.2-42. Fields Updated by Inquire.

Field	Tag
Patient Name	(0010,0010)
Patient ID	(0010,0020)
Patient Date of Birth	(0010,0030)
Patient Sex	(0010,0040)
Other Patient ID	(0010,1000)

Study Instance UID	(0020,000D)
Study ID	(0020,0010)
Study Date	(0008,0020)
Study Time	(0008,0030)
Accession Number	(0008,0050)
Referring Physician Name	(0008,0090)
Study Description	(0008,1030)
Procedure Code Sequence	(0008,1032)
> Code Value	(0008,0100)
> Code Meaning	(0008,0104)
> Coding Scheme Designator	(0008,0102)
> Coding Scheme Version	(0008,0103)
Physician of Record Names	(0008,1048)
Performing Physician Name	(0008,1050)
Reading Physician Names	(0008,1060)
Series Instance UID	(0020,000E)
Body Part Examined	(0018,0015)
Request Attribute Sequence	(0040,0275)
> Scheduled Procedure Step Id	(0040,0009)
> Requested Procedure Id	(0040,1001)
> Requested Procedure Code SQ	(0032,1064)
>> Code Value	(0008,0100)
>> Code Meaning	(0008,0104)
>> Coding Scheme Designator	(0008,0102)
>> Coding Scheme Version	(0008,0103)

4.2.5.3.1.4. Response Status Handling

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**, handling of CStore SOP Class specific result statuses are handled as described in **Table 4.2-43**. If the Storage Association is in response to a CMove request, and it is unexpectedly closed before a CStore Response is received for the last image, Inquire will Abort the originating CMove Association. If the Storage Association is unexpectedly closed during the Release cycle (i.e. after the last image has been sent) the associated CMove command will be completed as normal.

Table 4.2-43. Inquire Response Behaviour for Store to Remote AE Request.

Status	Further Meaning	Error Code	Behaviour
Refused	Out of Resources	A700 – A7FF	Failure will be logged and reported to CMove Requestor. Subsequent CStores will continue, Association will be released normally. No further unsolicited Routing Jobs to Target AE will be attempted for 10 minutes.
Error	Data Set does not match SOP Class	A900 – A9FF	Failure will be logged and reported to CMove Requestor. Subsequence CStores will continue, Association will be released normally.
Error	Cannot Understand	Cxxx	
Warning	Coercion of Data Elements	B000	Image transmission considered successful; warning message logged at higher log levels.
Warning	Elements Discarded	B006	
Warning	Data Set does not match SOP Class	B007	
Success	Success	0000	Success / Warning count reported to CMove requestor in progress messages.

4.2.5.3.2. Activity: Initiate Storage Commitment (Push-Model) to Request Transfer of long-term ownership of Composite Objects to Remote AE

4.2.5.3.2.1. Description and Sequencing of Activities

InQuire will initiate a new Association when the InSight System wishes to transfer long-term ownership of a set of Composite Objects to the system associated with the Remote AE, where the Composite Objects have previously been successfully CStored to that system. It may send multiple Storage Commitment Requests over the Association, releasing the Association when there are no further requests to Action.

4.2.5.3.2.2. Proposed Presentation Contexts

When establishing an Association for Storage Commitment, InQuire will propose a single Presentation Context:

Table 4.2-44. Proposed Presentation Contexts by InQuire.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Storage Commitment Push Model	1.2.840.10008.5.1.20.1	Implicit Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

4.2.5.3.2.3. SOP Specific Conformance for Storage Commitment SOP Class

4.2.5.3.2.3.1. Storage Commitment Operations (N-ACTION)

InQuire may request Storage Commitment for any of the Composite Object SOP Classes that it supports as a CStore SCU (see **Table 4.2-37**).

Once successfully issued, the Transaction UID for the storage commitment remains valid indefinitely until a notification is received for the transaction. In the event of an error return from the Remote AE in response to the Storage Commitment N-ACTION invocation, the SOP Instances in the request will be retried at a later time with a new Transaction UID.

The Storage Media File-Set ID and UID Attributes will not be present in the N-Action message.

4.2.5.3.2.3.2. Storage Commitment Notifications (N-EVENT-REPORT)

InQuire can receive N-EVENT-REPORT notifications on an Association that it has initiated with the remote AE where a Presentation Context for the Storage Commitment Push Model has been successfully negotiated.

The behaviour of InQuire on receiving an N-EVENT-REPORT is summarised in the following table:

Table 4.2-45. InQuire Storage Commitment N-EVENT-REPORT Behaviour.

Event Type Name	Event Type Id	Behaviour
Storage Commitment Request Successful	1	The Referenced SOP Instances under Referenced SOP Sequence (0008,1199) are marked in the InSight System as safely Archived, and become candidates for deletion from local storage when resources are required for new imaging. The least recently accessed imaging will be deleted first.
Storage Commitment Request Complete – Failures Exist	2	The Referenced SOP Instances under Referenced SOP Sequence (0008,1199) are treated as in the success case above. The Referenced SOP Instances under Failed SOP Sequence (0008,1198) are individually logged as failed along with the transaction uid and failure code. These SOPs remain in the pending commitment list for later retry, but are not marked as safely archived, and will not become deletion candidates at this point.

Following Successful Storage Commitment and subsequent deletion, the InSight system may in the future re-retrieve the SOPs from the remote storage via a CMove request to the indicated Retrieve AE Title (0008,0054) when activity is next detected for the patient (eg a Booking is made in the enterprise information system) where the deleted study is likely to be relevant, based on configurable rules in the system such as matching or similar body part, modality, procedure code etc.

Inquire may return the following Status Codes in an N-EVENT-REPORT response:

Table 4.2-46. Inquire Storage Commitment N-EVENT-REPORT Response Status Reasons.

Service Status	Further Meaning	Error Code	Behaviour
Success	Success	0000	The Storage Commitment result has been successfully processed
Failure	No Such Event Type	0113H	Event Id not 1 or 2 in N-EVENT-REPORT request
	Invalid Argument Value	0115H	Transaction UID (0008,1195) is missing or empty, or neither the Reference SOP Sequence (0008,1199) nor Failed SOP Sequence (0008,1198) are populated. Offending Element List (0000,0901) will be populated to indicate which fields are missing
	Processing Failure	0110H	An internal error occurred while notifying the InSight System of the Storage Commitment Notification

4.2.5.3.3. Activity: Send IOCM KOS Object

4.2.5.3.3.1. Description and Sequencing of Activities

In the InSight System, images may be removed from a study due to: Image Quality; Incorrect Parameters (e.g. view code, laterality etc.); or Incorrect Procedure Step. If any part of the affected study has already been sent to a separate long-term storage node, then an IOCM Rejection Note KOS Document is generated and sent to each long-term storage node which has received any part of the study to indicate the affected SOP Instances have been removed from the study. This may happen before or after a Storage Commitment request has been issued to the storage node for any part of the study.

4.2.5.3.3.2. Proposed Presentation Contexts

Table 4.2-47. Presentation Contexts Proposed by Inquire for IOCM KOS Object.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Key Object Selection Document	1.2.840.10008.5.1.4.1.1.88.59	Implicit Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

4.2.5.3.3.3. SOP Specific Conformance for Storage of IOCM KOS Object

Any failure detected during the send of an IOCM KOS object is reported to the InSight System, which will flag the error to System Administrators.

4.2.5.4. Association Acceptance Policy

4.2.5.4.1. Activity: Handling Query / Retrieve Requests and Storage Commitment Notifications from Remote AEs

4.2.5.4.1.1. *Description and sequencing of Activities*

When Inquire accepts an Association with one or more Presentation Contexts for supported Query/Retrieve SOP Classes as SCP, or the Storage Commitment SOP Class as SCU, the remote Application Entity can send any number of CEcho, CFind or CMove Requests, or Storage Commitment N-Event-Report Notifications, to which Inquire will respond as appropriate; the remote Application Entity is expected to release the Association when no further commands are to be sent.

When processing a CFind request, the resulting InSight Database query will run to completion before any normal responses are sent; depending on the specified Matching Keys, some queries will take longer than others. If a C-CANCEL-FIND-RQ is received while the Database Query is in progress or while matches are being sent, a final response with the status Cancelled will be sent immediately. The Association can then be released, or further Query/Retrieve requests sent as required by the SCU.

When processing a CMove request, Inquire initiates the Association to the CMove Destination on a separate thread. Once this Association is established successfully, Inquire will send progress messages to the CMove SCU when each CStore completes if a progress message hasn't been sent for at least 1000ms. Once the CStore Association is established, if a C-CANCEL-MOVE-RQ is received Inquire will finish sending the current CStore command, release the Association with the CStore Destination and send a CMove response with status Cancelled to the CMove SCU. The Association can then be released by the Requestor, or further Query/Retrieve requests sent as required by the SCU.

When processing a Storage Commitment N-Event-Report Notification, the Remote AE can send any number of Storage Commitment N-EVENT-REPORT notifications for outstanding Storage Commitment Transactions over that association. Inquire will report the SOP Success and Failures for the transaction, then mark the transaction as complete in the InSight system. It is expected that the Association Requestor will release the association when it has no further Transactions to notify.

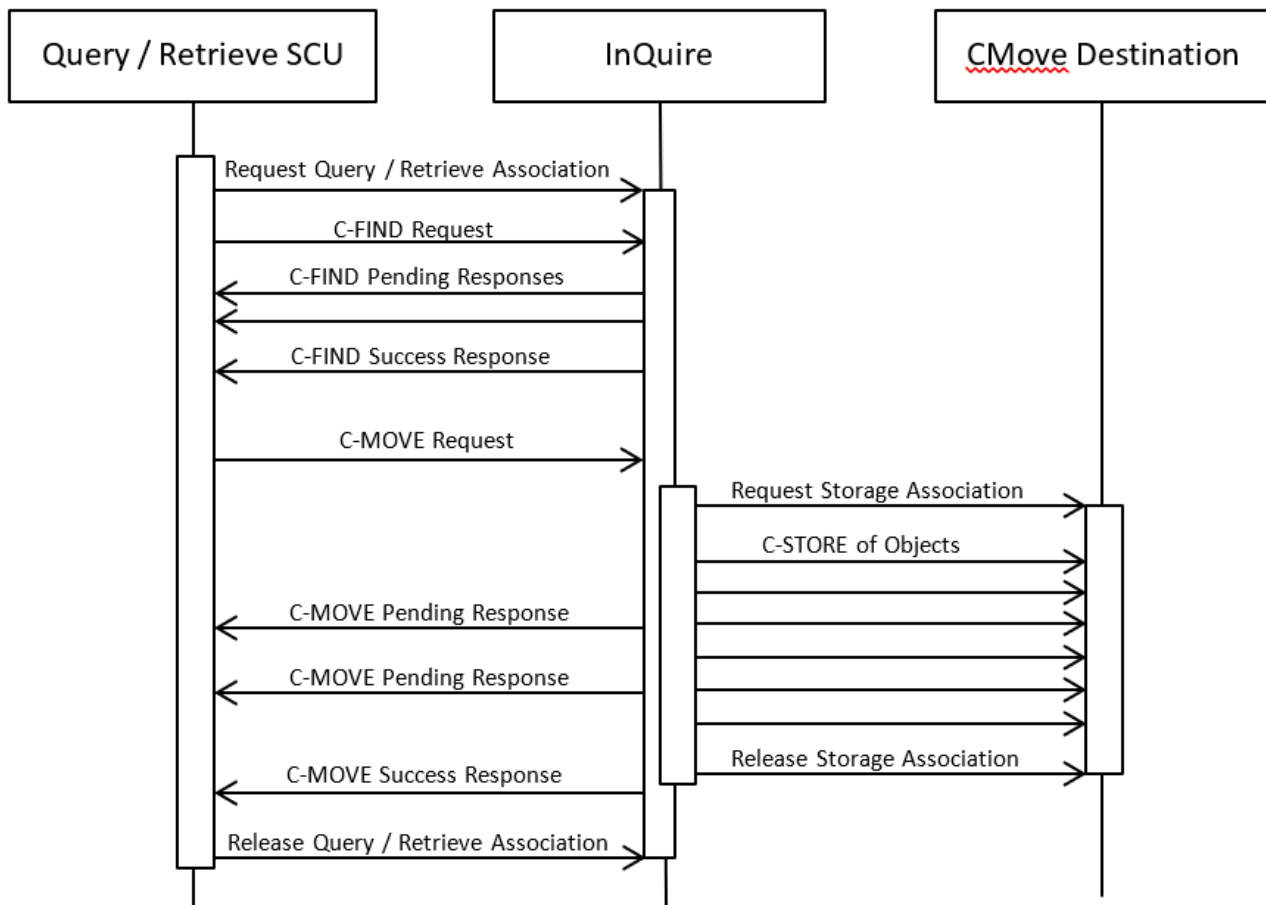


Figure 4.2-2. Sequencing of Activity: Query / Retrieve.

4.2.5.4.1.2. Accepted Presentation Contexts

Inquire will accept Presentation Contexts for the Abstract Syntax / Transfer Syntax combinations listed in **Table 4.2-48**. Note that all Transfer Syntaxes are acceptable for the Verification SOP Class as there is no Information Object associated with the Service. Where multiple Transfer Syntaxes are offered in a Presentation Context for a given Abstract Syntax in the Association Request, the first supported Transfer Syntax will be selected for that Presentation Context.

Table 4.2-48. Accepted Presentation Contexts by Inquire.

Abstract Syntax		Transfer Syntax		Role	Ext. Neg.
Name	UID	Name	UID		
Verification	1.2.840.10008.1.1	Any		SCP	None
Storage Commitment Push Model	1.2.840.10008.5.1.20.1	Implicit Little Endian	1.2.840.10008.1.2	SCU	None
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		
Query / Retrieve Information Model SOP Classes from Table 4.2-37	See Table 4.2-37	Implicit Little Endian	1.2.840.10008.1.2	SCP	See Note
		Explicit Little Endian	1.2.840.10008.1.2.1		
		Explicit Big Endian	1.2.840.10008.1.2.2		

Note: CFind Extended Negotiation – Inquire does not support Relational Queries or combined date-time matching, but does supports fuzzy semantic matching on Person Name fields

4.2.5.4.1.3. SOP Specific Conformance for Verification Class

Inquire provides standard conformance to the Verification SOP Class as an SCP

4.2.5.4.1.4. SOP Specific Conformance for Query Service Classes

Inquire supports matching on the keys listed in **Table 4.2-49** to **Table 4.2-53**. Where a field is listed as Universal matching only and a value is supplied in the query, the value supplied will be ignored – i.e. these keys are supported for existence but not matching as per PS 3.4-C.2.2.1.3.

Inquire does not support Relational Queries or combined date and time matching, however when fuzzy-semantic Person Name matching has been successfully negotiated, the Patient Name field will be matched using standard Sybase soundex functionality. The Patient Name field is always treated as case-insensitive. If the Specific Character Set attribute (0008,0005) is present in the Query Data Set and set to Unicode UTF-8 (ISO_IR 192), affected strings will be converted to ISO Latin 1 if possible. In all other cases the Character Set is ignored and strings are assumed to be ISO Latin 1. In the Result Set the Specific Character Set attribute will be set to Latin 1 (ISO_IR 100) if and only a string in the result set contains a character outside the ASCII Default repertoire. Timezone Offset from UTC (0008,0201) are ignored and not included in the CFind Results Information Objects.

The values returned for a query may differ to the values present in the related Composite Object as originally received by InDigoX, as the InSight Database will always return the most up-to-date information as received from the Institution Information System, or as edited using the InSight System tools.

Table 4.2-49. Inquire Supported Patient Root & Patient / Study Only PATIENT Level Query Keys.

Name	Tag	Matching Type
Patient Name	(0010,0010)	Single Value, Wild Card, Universal
Patient ID	(0010,0020)	Single Value, Universal
Patient Date of Birth	(0010,0030)	Single Value, Range, Universal
Patient Sex	(0010,0040)	Single Value, Universal
Other Patient IDs	(0010,1000)	Single Value, Universal
Number of Patient Related Studies	(0020,1200)	Universal
Number of Patient Related Series	(0020,1202)	Universal
Number of Patient Related Instances	(0020,1204)	Universal
Retrieve AE Title	(0008,0054)	Inquire AE Title
Instance Availability	(0008,0056)	Universal

Table 4.2-50. Inquire Supported Patient Root & Patient / Study Only STUDY Level Query Keys.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value, Required
Study Instance UID	(0020,000D)	Single Value, Universal
Study Date	(0008,0020)	Single Value, Range, Universal
Study Time	(0008,0030)	Single Value, Range, Universal
Accession Number	(0008,0050)	Single Value, Wild Card, Universal
Study ID	(0020,0010)	Single Value, Wild Card, Universal
Modalities In Study	(0008,0061)	Single Value, Universal
Study Description	(0020,1030)	Universal
Referring Physician	(0008,0090)	Universal
Name of Physician(s) Reading Study	(0008,1060)	Universal
Number of Study Related Series	(0020,1206)	Universal
Number of Study Related Instances	(0020,1208)	Universal
Retrieve AE Title	(0008,0054)	Inquire AE Title
Instance Availability	(0008,0056)	Universal

Table 4.2-51. Inquire Supported Study Root STUDY Level Query Keys.

Name	Tag	Matching Type
Patient Name	(0010,0010)	Single Value, Wild Card, Universal
Patient ID	(0010,0020)	Single Value, Universal
Patient Date of Birth	(0010,0030)	Single Value, Range, Universal
Patient Sex	(0010,0040)	Single Value, Universal
Other Patient IDs	(0010,1000)	Single Value, Universal
Study Instance UID	(0020,000D)	Single Value, Universal
Study Date	(0008,0020)	Single Value, Range, Universal
Study Time	(0008,0030)	Single Value, Range, Universal
Accession Number	(0008,0050)	Single Value, Wild Card, Universal
Study ID	(0020,0010)	Single Value, Wild Card, Universal
Modalities In Study	(0008,0061)	Single Value, Universal
Study Description	(0020,1030)	Universal
Referring Physician	(0008,0090)	Universal
Name of Physician(s) Reading Study	(0008,1060)	Universal
Number of Study Related Series	(0020,1206)	Universal
Number of Study Related Instances	(0020,1208)	Universal
Retrieve AE Title	(0008,0054)	Inquire AE Title
Instance Availability	(0008,0056)	Universal

Table 4.2-52. Inquire Supported Patient Root and Study Root SERIES Level Query Keys.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value (Required If Patient Root)
Study Instance UID	(0020,000D)	Single Value Required
Modality	(0008,0060)	Single Value, Universal
Series Instance UID	(0020,000E)	Single Value, Universal
Series Number	(0020,0011)	Single Value, Universal
Series Description	(0008,103E)	Universal
Series Date	(0008,0021)	Universal
Series Time	(0008,0031)	Universal
Body Part Examined	(0018,0015)	Universal
Performing Physician	(0008,1050)	Universal
Patient Position	(0018,5100)	Universal
Frame Of Reference	(0020,0052)	Universal
Device Model	(0008,1090)	Universal
Laterality	(0020,0060)	Universal
Manufacturer	(0008,0070)	Universal
Request Attribute Sequence	(0040,0275)	Universal Sequence
> Accession Number	(0008,0050)	Universal
> Study Instance UID	(0020,000D)	Universal
> Requested Procedure Id	(0040,1001)	Universal
> Scheduled Procedure Step Id	(0040,0009)	Universal
> Scheduled Procedure Step Description	(0040,0007)	Universal
> Requested Procedure Code Sequence	(0032,1064)	Universal Sequence
>> Code Value	(0008,0100)	Universal
>> Code Meaning	(0008,0104)	Universal
>> Coding Scheme Designator	(0008,0102)	Universal
>> Coding Scheme Version	(0008,0103)	Universal
Number of Series Related Instances	(0020,1209)	Universal
Retrieve AE Title	(0008,0054)	Inquire AE Title
Instance Availability	(0008,0056)	Universal

Table 4.2-53. InQUIRE Supported Patient Root and Study Root IMAGE Level Query Keys.

Name	Tag	Matching Type
Patient ID	(0010,0020)	Single Value (Required if Patient Root)
Study Instance UID	(0020,000D)	Single Value Required
Series Instance UID	(0020,000E)	Single Value Required
SOP Instance UID	(0008,0018)	Single Value, Universal
Instance Number	(0020,0013)	Single Value, Universal
SOP Class UID	(0008,0016)	Universal
Content Date	(0008,0023)	Universal
Content Time	(0008,0033)	Universal
Acquisition Date	(0008,0022)	Universal
Acquisition Time	(0008,0032)	Universal
Slice Thickness	(0018,0050)	Universal
Image Type	(0008,0008)	Universal
Retrieve AE Title	(0008,0054)	InQUIRE AE Title
Instance Availability	(0008,0056)	Universal

InQUIRE reserves the right to refuse a query which will generate too many results, for example supplying just a Patient Name as “A*”. In particular the Study Date range is limited to 1 month if no other matching fields are supplied. A Study Time Range will be ignored unless a Study Date (Single Value or Range) is supplied. However, if the query is not refused, then all matches will be returned irrespective of number.

A Query request will result in responses with the following status codes:

Table 4.2-54. InQUIRE Query Response Status Reasons.

Service Status	Further Meaning	Error Code	Reasons
Failure	Identifier Does Not Match SOP Class	A900	The Identifier was missing or could not be interpreted as an Information Object for the Query SOP Class at the given level. Error Comment (0000,0902) will be populated with details
	Unable to Process	C000	The InSight Database query to retrieve the matches failed or was refused. Full details will be logged in the InQUIRE error log. Error Comment (0000,0902) will be populated with details
Cancelled	Matching terminated due to Cancel Request	FE00	The Cancelled status will be set on the next response returned after receiving the Cancel Request
Success	Matching is complete	0000	All Pending matches have been sent
Pending	Matches are continuing – all requested Optional Keys were supported	FF00	Response contains an Information Object representing the match containing all requested keys
	Matches are continuing – Warning that one or more Optional Keys were not supported for existence for this identifier	FF01	Response contains an Information Object representing the match, but some requested optional keys are not supported - these are logged in the InQUIRE error log

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**.

4.2.5.4.1.5. *SOP Specific Conformance for Retrieve Service Classes*

InQUIRE supports Relational Retrieve – if it is successfully negotiated, only UIDs at the requested Query/Retrieve Level need be supplied, irrespective of the SOP Class used for the request. InQUIRE supports retrieval of a list of UIDs.

Inquire may generate CStore commands in response to the CMove request for the SOP Classes listed in section **4.2.5.3 Association Initiation Policy**. As described in that section, the SOP Instances will be updated as they are sent with the latest Hierarchy and Volatile Demographic information.

If the CStore Association is aborted by the CMove Destination or otherwise unexpectedly terminated, the Query Retrieve association itself will be aborted.

A CMove request will generate Responses with the following statuses:

Table 4.2-55. Inquire Retrieve Response Status Reasons.

Service Status	Further Meaning	Error Code	Reasons
Failure	Unable to Calculate Matches	A701	The InSight System could not calculate the set of SOP Instances for the requested hierarchy level, or the set of SOP Instances exist on the InSight System, but Inquire is unable to retrieve them. Error Comment (0000,0902) will be populated.
	Move Destination Unknown	A801	The current Inquire configuration does not include details of the specified CMove destination
	Identifier Does Not Match SOP Class	A900	The Identifier was missing or could not be interpreted as an Information Object for the Retrieve SOP Class at the given level. Error Comment (0000,0902) will be populated with details
	Unable to Process	C000	The InSight Database query to retrieve volatile data for the SOP Instances failed, or Inquire failed to initiate a CStore association with the CMove Target, even though it is known. Full details will be logged in the Inquire error log. Error Comment (0000,0902) will be populated.
Cancelled	Matching terminated due to Cancel Request	FE00	The Cancelled status will be set on the next response returned after receiving the Cancel Request
Success	Sub-operations Complete – No Failures	0000	All CStore sub-operations completed with Success or Warning status
Warning	Sub-operations Complete – One or more Failures	B000	All CStore sub-operations completed, some returned Failure status. Failed SOP Instance UID List (0008,0058) will be populated
Pending	Sub-operations are continuing	FF00	CStore sub-operations are progressing, sent at most once every 1000ms

The handling of terminal communication errors and normal Association release are detailed in section **4.2.1.3 Association Termination**. If the CMove Association is unexpectedly terminated, the CStore Association will be Aborted.

4.2.5.4.1.6. *SOP Specific Conformance for Storage Commitment SOP Class*

When a Storage Commitment notification is received on an Association initiated by a remote peer, it is handled in exactly the same way as when the notification is received on an Association initiated by Inquire, see **Section 4.2.5.3.2.3.2 Storage Commitment Notifications (N-EVENT-REPORT)** under **4.2.5.3.2 Activity: Initiate Storage Commitment (Push-Model) to Request Transfer of long-term ownership of Composite Objects to Remote AE**.

4.3. Network Interfaces

4.3.1. Physical Network Interface

The InSight DICOM Application Entities use the WinSock 2 Berkeley Socket API to interact with TCP/IP sockets. As such they are independent of the Physical Network - it is likely within a hospital that the network will be 100baseT or Gigabit Ethernet, but this is not a requirement.

The hardware hosting the Departmental Server node may have multiple network adaptors and IP Addresses, which may be fixed or allocated by DHCP. However, in order to be reachable by the Remote AEs, these IP addresses must be predictable so in the case of DHCP the Departmental Server node will require a permanent address lease. By the nature of Windows Sockets, the Dicom Application Entities will be reachable on their configured ports on all IP Addresses allocated to the node.

4.3.2. Additional Protocols

No particular protocols are used by the Application Entities.

4.3.3. IPv4 and IPv6

The InSight DICOM Application Entities only support IPv4 addresses.

4.4. Configuration

4.4.1. AE Title / Presentation Address Mapping

4.4.1.1. Local AE Titles

The mapping from Application Entity to AE Title and TCP / IP port is configurable via the InSight System tools. When a new Departmental Server instance is installed on an InSight PACS, the Application Entities are pre-allocated default AE Titles and TCP/IP ports as shown in the table below, where the <n> in the AE Titles is a counter, as there may be multiple Departmental Server nodes in the system.

Table 4.4-1. Default Application Entity Title Configuration.

Application Entity	Default AE Title	Default TCP/IP Port
InList	INLIST<n>	3001
InDigoX	INDIGOX<n>	104
InPort	INPORT<n>	None
InQuire	INQUIRE<n>	3000

4.4.1.2. Remote AE Title / Presentation Address Mapping

The TCP/IP address or hostname and port and the set of offered and provided DICOM services for each Remote AE are configurable via the InSight System Tools. A number of IP Addresses / ports can be assigned to a given Remote AE to allow connections from Application Entities hosted on multi-homed servers. Connections are only allowed from AE Titles presenting on one of their known IP Addresses, or an IP Address retrieved from the DNS for the configured hostname.

Each InSight Application Entity can be configured to accept / be able to initiate associations with a subset of the configured Remote AEs. For each InSight / Remote AE Pairing, a subset of the Remote AE's supported Abstract Syntaxes can be selected, along with a subset of Transfer Syntaxes that are known to be compatible.

Only presentation contexts that are configured for a given InSight AE / Remote AE will be accepted or offered on an association between those two entities.

4.4.2. Parameters

The following table lists parameters that are configurable. Generally this is performed through the InSight System tools for each Application Entity. Where the MaxPDU sendable is configurable, this is via a registry key for each Application Entity on the Departmental Server.

Table 4.4-2. Application Entity Configuration.

Parameter	Configurable	Default	Note
General Parameters			
Maximum PDU size receivable	No	Unlimited	Will accept whatever is offered
Timeout waiting for TCP/IP connect() response	No	2500ms	
Timeout waiting for A-ASSOCIATE-RQ PDU after TCP/IP connection opened (ARTIM)	Yes	5000ms	Globally configured per Remote AE
Timeout waiting for response to Association Request	No	Infinite	
Timeout waiting for expected data within a message exchange	No	Infinite	
InList			
Maximum PDU size sendable	Yes	0	Unlimited, Configured via registry key
Maximum number of Simultaneous Associations	Yes	5	
Remote AE Titles	Yes		AE Title, IP address, Port
Supported Abstract Syntaxes	Yes		Configured Per Remote AE
Supported Transfer Syntaxes	Yes		Configured Per Remote AE
InDigoX			
Maximum PDU size sendable	Yes	0	Unlimited, Configured via registry key
Maximum number of Simultaneous Associations	Yes	5 Accept 1 Request	
Remote AE Titles	Yes		AE Title, IP address, Port
Supported Abstract Syntaxes	Yes		Configured Per Remote AE
Supported Transfer Syntaxes	Yes		Configured Per Remote AE
InPort			
Maximum PDU size sendable	Yes	0	Unlimited, Configured via registry key
Maximum number of Simultaneous Associations	Yes	1 Query 5 Retrieve	Number of Retrieve Associations is configurable
CFind Source	Yes		One Remote AE is nominated as the CFind Source
CStore Target	Yes		AE Title of the InDigoX instance
Remote AE Titles	Yes		AE Title, IP address, Port
Supported Abstract Syntaxes	Yes		Configured Per Remote AE
Supported Transfer Syntaxes	Yes		Configured Per Remote AE
InQuire			
Maximum PDU size sendable	Yes	0	Unlimited, Configured via registry key
Maximum number of Simultaneous Associations	Yes	5 Accept 5 Request	5 Query / Retrieve Associations, 5 resultant Storage Associations
Maximum number of simultaneous unsolicited routing Associations	Yes	10	
Remote AE Titles	Yes		AE Title, IP address, Port

Supported Abstract Syntaxes	Yes		Configured Per Remote AE
Supported Transfer Syntaxes	Yes		Configured Per Remote AE

5. Media Interchange

The InSight DICOM Application Entities specified in this document do not support Media Interchange.

6. Support of Character Sets

The InSight DICOM Application Entities specified in this document support Specific Character Sets as follows:

Objects are stored as received by the CStore SCP, with the Specific Character Set attribute (0008,0005) preserved and all string encodings preserved. Where string values are extracted from a CStore or Query data set by the relevant SCP for use in processing, the character set ISO Latin 1 (ISO_IR 100) is assumed. If the Specific Character Set is UTF8 (ISO_IR 192), a conversion to ISO_IR 100 is performed if possible.

When a Composite Object, Query Request or Query Response is created or updated, all strings in the Data Set are analysed and if only characters from the default repertoire are present, the Specific Character Set element (0008,0005) will not be present in the data set. If all characters can be represented in the ISO Latin 1 character set, then Specific Character Set will be present with the single value 'ISO_IR 100'. Otherwise, all strings in the Data Set (including private elements if the object was originally received in an Explicit syntax where the VRs are known) will be converted as necessary to UTF_8 and Specific Character Set will be present with the single value 'ISO_IR 192'.

7. Security

7.1. Security Profiles

Security Profiles are not supported.

7.2. Association Level Security

Each Application Entity which listens on its configured TCP/IP Port for an incoming network connection (InList, InDigoX and InQuire) has a configured list of remote Application Entities, together with their Host Name or set of IP addresses, from which it may accept connections. If a connection is detected from an IP address not in the configured list or that is not returned by the DNS for any peer hostnames, the first Association Request will result in the Association being Rejected with the reason "Calling AE Title Not Recognized", and a message being logged with the InSight database. Subsequent connections from that IP address will result in the socket being closed immediately with no attempt at association negotiation.

If the connection is from an IP address which hosts known Remote AEs, but the Calling AE Title in the Association Request does not match an AE Title configured for that IP Address, the Association will be rejected with the reason "Calling AE Title Not Recognized", even if the AE Title is known on a different IP Address.

7.3. Application Level Security

The DICOM Application Entities are implemented as Windows Services. As such they have no direct User interaction, so further direct User related security is not required. Where User input is utilised indirectly it is via data input through other application User Interfaces to the Database. Each of these Applications has its own user authentication methods outside the scope of this document, and all user input is filtered, validated and encoded

by those applications before it is passed to the Database for use by the Application Entities detailed in this document.

8. Annexes

8.1. IOD Contents

8.1.1. Created SOP Instances

The following tables use the following abbreviations:

"Presence of ..." column:

- **VNAP** Value Not Always Present (attribute sent zero length if no value is present)
- **ANAP** Attribute Not Always Present
- **ALWAYS** Attribute Always Present with Value
- **EMPTY** Attribute is sent without a value

"Source" column:

- **SYSTEM** the attribute value is sourced from the Patient / Study hierarchy in the InSight System
- **USER** the attribute value is sourced from User input
- **AUTO** the attribute value is generated automatically by the creating application

Note:

All dates and times are encoded in the local configured calendar and time.

8.1.1.1. Greyscale Softcopy Presentation State IOD Modules

Presentations for Greyscale Images saved within the InSight System will be expressed to external systems as Greyscale Softcopy Presentation State objects.

Table 8.1-1. IOD of Created Greyscale Softcopy Presentation State SOP Instances.

IE	Module	Reference	Presence of Module
Patient	Patient	Error! Reference source not found.	ALWAYS
Study	General Study	Error! Reference source not found.	ALWAYS
Series	General Series	Error! Reference source not found.	ALWAYS
	Presentation Series	Error! Reference source not found.	ALWAYS
Equipment	General Equipment	Error! Reference source not found.	ALWAYS
Presentation State	Presentation State Identification	Error! Reference source not found.	ALWAYS
	Presentation State Relationship	Error! Reference source not found.	ALWAYS
	Presentation State Shutter	Error! Reference source not found.	Only if Shutter Applied
	Display Shutter	Error! Reference source not found.	Only if Shutter Applied
	Overlay Activation	Error! Reference source not found.	Only if Overlays Present in Referenced Image Headers

	Display Area	Error! Reference source not found.	ALWAYS
	Graphic Annotation	Error! Reference source not found.	Only if Annotations Applied
	Spatial Transformation	Error! Reference source not found.	ALWAYS
	Graphic Layer	Error! Reference source not found.	Only if Annotations Applied
	Modality LUT	Error! Reference source not found.	ALWAYS
	Softcopy VOI LUT	Error! Reference source not found.	ALWAYS
	Softcopy Presentation LUT	Error! Reference source not found.	ALWAYS
	SOP Common	Error! Reference source not found.	ALWAYS

8.1.1.2. Colour Softcopy Presentation State IOD Modules

Presentations for Colour Images saved within the InSight System will be expressed to external systems as Colour Softcopy Presentation State objects.

Table 8.1-2. IOD of Created Colour Softcopy Presentation State SOP Instances.

IE	Module	Reference	Presence of Module
Patient	Patient	Error! Reference source not found.	ALWAYS
Study	General Study	Error! Reference source not found.	ALWAYS
Series	General Series	Error! Reference source not found.	ALWAYS
	Presentation Series	Error! Reference source not found.	ALWAYS
Equipment	General Equipment	Error! Reference source not found.	ALWAYS
Presentation State	Presentation State Identification	Error! Reference source not found.	ALWAYS
	Presentation State Relationship	Error! Reference source not found.	ALWAYS
	Presentation State Shutter	Error! Reference source not found.	Only if Shutter Applied
	Display Shutter	Error! Reference source not found.	Only if Shutter Applied
	Overlay Activation	Error! Reference source not found.	Only if Overlays Present in Referenced Image Headers
	Display Area	Error! Reference source not found.	ALWAYS
	Graphic Annotation	Error! Reference source not found.	Only if Annotations Applied
	Spatial Transformation	Error! Reference source not found.	ALWAYS
	Graphic Layer	Error! Reference source not found.	Only if Annotations Applied
	ICC Profile	Error! Reference source not found.	ALWAYS
	SOP Common	Error! Reference source not found.	ALWAYS

8.1.1.3. Spatial Registration IOD Modules

Table 8.1-3. IOD of Created Spatial Registration SOP Instances.

IE	Module	Reference	Presence of Module
Patient	Patient	Error! Reference source not found.	ALWAYS
Study	General Study	Error! Reference source not found.	ALWAYS
Series	General Series	Error! Reference source not found.	ALWAYS
	Spatial Registration Series	Error! Reference source not found.	ALWAYS
Frame of Reference	Frame of Reference	Error! Reference source not found.	ALWAYS
Equipment	General Equipment	Error! Reference source not found.	ALWAYS
Spatial Registration	Spatial Registration	Error! Reference source not found.	ALWAYS
	Common Instance Reference	Error! Reference source not found.	ALWAYS
	SOP Common	Error! Reference source not found.	ALWAYS

8.1.1.4. IOCM Rejected Image Note KOS IOD Modules

When images are rejected or reassigned in the InSight PACS, IOCM KOS Documents will be generated and sent to any CStore target to which the study has been sent and a Storage Commitment request made.

Table 8.1-4. IOD of Created Rejection Note KOS Document SOP Instances.

IE	Module	Reference	Presence of Module
Patient	Patient	Error! Reference source not found.	ALWAYS
Study	General Study	Error! Reference source not found.	ALWAYS
Series	Key Object Document Series	Error! Reference source not found.	ALWAYS
Equipment	General Equipment	Error! Reference source not found.	ALWAYS
Document	Key Object Document	Error! Reference source not found.	ALWAYS
	SR Document Content	Error! Reference source not found.	ALWAYS
	SOP Common	Error! Reference source not found.	ALWAYS

8.1.1.5. Basic Text Structured Report IOD Modules

Where Report Text has been received from the RIS via HL7, a Basic Text Structured Report conforming to the TID 2005 Transcribed Diagnostic Imaging Report Template.

Table 8.1-5. IOD of Created Basic Text Structured Report SOP Instances.

IE	Module	Reference	Presence of Module
Patient	Patient	Error! Reference source not found.	ALWAYS
Study	General Study	Error! Reference source not found.	ALWAYS
Series	SR Document Series	Error! Reference source not found.	ALWAYS
Equipment	General Equipment	Error! Reference source not found.	ALWAYS
Document	SR Document General	Error! Reference source not found.	ALWAYS
	SR Document Content	Error! Reference source not found.	ALWAYS
	SOP Common	Error! Reference source not found.	ALWAYS

8.1.1.6. Common Modules

Table 8.1-6. Patient Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Patient Name	(0010,0010)	PN	Values match the Patient Record held in the InSight System.	ALWAYS	SYSTEM
Patient ID	(0010,0020)	LO			
Patient Date of Birth	(0010,0030)	DA			
Patient Sex	(0010,0040)	CS			
Other Patient ID	(0010,1000)	LO		VNAP	

Table 8.1-7. General Study Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Study Instance UID	(0020,000D)	UI	Values match the Study Record held in the InSight System	ALWAYS	SYSTEM
Study ID	(0020,0010)	SH		ALWAYS	
Study Description	(0008,1030)	LO		ALWAYS	
Study Date	(0008,0020)	DA		ALWAYS	
Study Time	(0008,0030)	TM		ALWAYS	
Referring Physician Name	(0008,0090)	PN		VNAP	
Accession Number	(0008,0050)	SH		ALWAYS	
Procedure Code Sequence	(0008,1032)	SQ		ANAP	
> Code Value	(0008,0100)	SH		ALWAYS	
> Code Meaning	(0008,0104)	LO		ALWAYS	
> Coding Scheme	(0008,0102)	SH		ALWAYS	
> Coding Scheme Version	(0008,0103)	SH		VNAP	
Reading Physicians	(0008,1060)	PN		ANAP	
Physicians of Record	(0008,1048)	PN		ANAP	

Table 8.1-8. General Series Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
----------------	-----	----	-------	-------------------	--------

Series Instance UID	(0020,000E)	UI	Generated by Viewing Workstation / background server at time of Presentation / Spatial Registration Creation	ALWAYS	AUTO
Series Number	(0020,0011)	IS	1		
Modality	(0008,0060)	CS	Specialised by SOP Class		
Series Date	(0008,0021)	DA	Date of Export		
Series Time	(0008,0031)	TM	Time of Export		

Table 8.1-9.General Equipment Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Manufacturer	(0008,0070)	LO	InSight Medical Systems Ltd	ALWAYS	AUTO
Software Version	(0018,1020)	LO	Will Match InQuire Implementation Version Name in <i>Table 3.8-40</i>		
Manufacturers Model Name	(0008,1090)	LO	InQuire		

8.1.1.7. Presentation State Modules

Table 8.1-10. Presentation Series Module of Created Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	PR	ALWAYS	AUTO

Table 8.1-11. SOP Common Module of Created Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.11.1 (Greyscale) 1.2.840.10008.5.1.4.1.1.11.2 (Colour)	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by Viewing Workstation at time of Presentation Creation		
Instance Creation Date	(0008,0012)	DA	Date of Presentation Export		
Instance Creation Time	(0008,0013)	TM	Time of Presentation Export		

Table 8.1-12. Presentation State Identification Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Presentation Creation Date	(0070,0082)	DA	Date of Presentation Creation on Viewing Workstation	ALWAYS	USER
Presentation Creation Time	(0070,0083)	TM	Time of Presentation Creation on Viewing Workstation	ALWAYS	USER
Instance Number	(0020,0013)	IS	1	ALWAYS	AUTO

Content Label	(0070,0080)	CS	User Selection from set of labels defined by Configuration in the InSight System	ALWAYS	USER
Content Description	(0070,0081)	LO	As Entered by Workstation User	VNAP	USER
Content Creator's Name	(0070,0084)	PN	Workstation User at time of Presentation Creation	VNAP	USER

Table 8.1-13. Presentation State Relationship Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Referenced Series Sequence	(0008,1115)	SQ	One or More Items	ALWAYS	SYSTEM
> Series Instance UID	(0020,000E)	UI	From Referenced Images		
> Referenced Image Sequence	(0008,1140)	SQ	One or More Items		
>> Referenced SOP Class UID	(0008,1150)	UI	From Referenced Image		
>> Referenced SOP Instance UID	(0008,1155)	UI	From Referenced Image		
>> Referenced Frame Number	(0008,1160)	IS	May be Multi-valued. If not present, All Frames are referenced	ANAP	

Table 8.1-14. Presentation State Shutter Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Shutter Presentation Value	(0018,1622)	US	Black (0000H)	ALWAYS	AUTO
Shutter Presentation Colour CIE Lab Value	(0018,1624)	US	Black, only present in Colour Presentation State	ANAP	AUTO

Table 8.1-15. Display Shutter Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Shutter Shape	(0018,1600)	CS	RECTANGULAR	ALWAYS	USER
Shutter Left Vertical Edge	(0018,1602)	IS	Bounds of Rectangular Shutter as inherited from image or applied by User at time of Presentation Creation		
Shutter Right Vertical Edge	(0018,1604)	IS			
Shutter Upper Horizontal Edge	(0018,1606)	IS			
Shutter Lower Horizontal Edge	(0018,1608)	IS			

Table 8.1-16. Overlay Activation Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Overlay Activation Layer	(60xx,1001)	CS	Attribute will be present if the given Group 60xx Overlay is present in the Referenced Image Header. Value will be OVERLAY if the given overlay group was selected for display by the user when the Presentation was saved, otherwise the Value will not be present.	VNAP	USER

Table 8.1-17. Presentation Item Application Macro Attributes.

Attribute Name	Tag	VR	Value	Presence of Value	Source
----------------	-----	----	-------	-------------------	--------

Referenced Image Sequence	(0008,1140)	SQ	The SOP Instance to which the Presentation Item applies.	ALWAYS	SYSTEM
> Referenced SOP Class UID	(0008,0016)	UI			
> Referenced SOP Instance UID	(0008,0018)	UI			
> Referenced Frame Number	(0008,1160)	IS	Not present if item applies to all frames of this SOP Instance	ANAP	

Table 8.1-18. Display Area Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Displayed Area Selection SQ	(0070,005A)	SQ		ALWAYS	AUTO
> Include Error! Reference source not found. "Presentation Item Application Macro"			If not present, this sequence item applies to all SOP Instances of the Presentation State Relationship Module	ANAP	SYSTEM
> Pixel Origin Interpretation	(0048,0301)	CS	FRAME	ALWAYS	AUTO
> Displayed Area Top Left Hand Corner	(0070,0052)	SL	The top left pixel (after spatial transformation) of the displayed image(s), given as column\row where column is the horizontal offset (X) and row is the vertical offset (Y) relative to the origin (1/1) of the pixel data <i>before spatial transformation</i>	ALWAYS	USER
> Displayed Area Bottom Right Hand Corner	(0070,0053)	SL	The bottom right pixel after spatial transformation, given as column/row relative to the origin as defined above	ALWAYS	USER
> Presentation Size Mode	(0070,0100)	CS	SCALE TO FIT MAGNIFY TRUE SIZE	ALWAYS	USER
> Presentation Pixel Spacing	(0070,0101)	DS	Given as row/column in mm. Will be present if Presentation Size Mode is TRUE SIZE , may be present otherwise. Taken from Pixel Spacing or calculated from Image Pixel Spacing & Magnification Factors if present in image header, or from User Calibration of image	ANAP	AUTO / USER
> Presentation Aspect Ratio	(0070,0102)	IS	Given as row/column. Present if Presentation Pixel Spacing (0070,0101) not present	ANAP	AUTO
> Presentation Pixel Magnification Ratio	(0070,0103)	FL	Present if Presentation Size Mode (0070,0100) is MAGNIFY	ANAP	USER

Table 8.1-19. Graphic Annotation Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Graphic Annotation Sequence	(0070,0001)	SQ	If Module is present, the sequence will contain at least one item	ALWAYS	USER
> Include Table 8.1-17. Presentation Item Application Macro Attributes.			If not present, this sequence item applies to all SOP Instances of the Presentation State Relationship Module	ANAP	SYSTEM
> Graphic Layer	(0070,0002)	CS	TAPE	ALWAYS	AUTO

			TEXT MEASUREMENT ROI COBB_ANGLE ANNOTATION MIN_MAX HIP_DISPLASIA CT_RATIO PARALLEL_MEASURE PERP_ANGLES ALPHA_ANGLE		
> Text Object Sequence	(0070,0008)	SQ	Text associated with this annotation. 0-n items may be present	ANAP	USER
>> Bounding Box Annotation Units	(0070,0003)	CS	PIXEL Present if Bounding Box is Present	ANAP	AUTO
>> Anchor Point Annotation Units	(0070,0004)	CS	PIXEL Present if Anchor Point is Present	ANAP	AUTO
>> Unformatted Text Value	(0070,0006)	ST		ALWAYS	USER
>> Bounding Box Top Left Hand Corner	(0070,0010)	FL	X/Y pair. Present if Anchor Point absent, may be present otherwise	ANAP	USER
>> Bounding Box Bottom Right Hand Corner	(0070,0011)	FL	X/Y pair. Present if Anchor Point absent, may be present otherwise	ANAP	USER
>> Bounding Box Text Horizontal Justification	(0070,0012)	CS	CENTER Present if Bounding Box present	ANAP	AUTO
>> Anchor Point	(0070,0014)	FL	X/Y pair. Present if Bounding Box absent, may be present otherwise	ANAP	USER
>> Anchor Point Visibility	(0070,0015)	CS	Y or N Present if Anchor Point present	ANAP	USER
> Graphic Object Sequence	(0070,0009)	SQ	Graphic associated with this annotation, zero or one item	ANAP	USER
>> Graphic Annotation Units	(0070,0005)	CS	PIXEL	ALWAYS	AUTO
>> Graphic Dimensions	(0070,0020)	US	2	ALWAYS	AUTO
>> Number of Graphic Points	(0070,0021)	US		ALWAYS	USER
>> Graphic Data	(0070,0022)	FL	Number of Graphics Points X/Y pairs	ALWAYS	USER
>> Graphic Type	(0070,0023)	CS	POLYLINE CIRCLE ELLIPSE	ALWAYS	USER
>> Graphic Filled	(0070,0024)	CS	Y if Graphic Layer (0070,0002) is TAPE N otherwise	ALWAYS	AUTO

Table 8.1-20. Spatial Transform Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Image Rotation	(0070,0042)	US	0, 90, 180 or 270 Clockwise rotation, to be applied before flip. For Mammography images, calculated automatically from View Code and Laterality to ensure Axilla is at top of displayed image	ALWAYS	USER / AUTO
Image Horizontal Flip	(0070,0041)	CS	Y or N.	ALWAYS	USER / AUTO

			For Mammography images, calculated automatically as above		
--	--	--	---	--	--

Table 8.1-21. Graphic Layer Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Graphic Layer Sequence	(0070,0060)	SQ		ALWAYS	AUTO
> Graphic Layer	(0070,0002)	CS	TAPE TEXT MEASUREMENT ROI COBB_ANGLE OVERLAY ANNOTATION MIN_MAX HIP_DISPLASIA CT_RATIO PARALLEL_MEASURE PERP_ANGLES ALPHA_ANGLE		
> Graphic Layer Order	(0070,0062)	IS	Lower numbered layers to be rendered first. TAPE is always layer 1 if present.		
> Graphic Layer Recommended Display Greyscale Value	(0070,0066)	US	Black (0000H) if Graphic Layer is TAPE , otherwise white (FFFFH)		
> Graphic Layer Recommended Display CIELab Value	(0070,0401)	US	White if Graphic Layer TEXT Black if Graphic Layer TAPE Otherwise Green (E147H/2828H/CACAH)		
> Graphic Layer Description	(0070,0068)	LO	Predefined description of the layer		

Table 8.1-22. Modality LUT Module of Created Greyscale Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality LUT Sequence	(0028,3000)	SQ	Taken from Image Header, single item if present and Rescale Details absent	ANAP	SYSTEM
> LUT Descriptor	(0028,3002)	US/SS	Taken from Image Header if present		
> LUT Explanation	(0028,3003)	LO			
> Modality LUT Type	(0028,3004)	LO			
> LUT Data	(0028,3006)	OW			
Rescale Intercept	(0028,1052)	DS	Taken from Image Header if present, otherwise 0 if Modality LUT Sequence not present		
Rescale Slope	(0028,1053)	DS	Taken from Image Header if present, otherwise 1 if Modality LUT Sequence not present		
Rescale Type	(0028,1054)	LO	Taken from Image Header if present, otherwise US (Unspecified) if Modality LUT Sequence not present		

Table 8.1-23. Softcopy VOI LUT Module of Created Greyscale Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Softcopy VOI LUT Sequence	(0028,3110)	SQ		ALWAYS	AUTO
> Include Error! Reference source not found. "Presentation Item Application Macro"			If not present, this sequence item applies to all SOP Instances of the Presentation State Relationship Module	ANAP	SYSTEM
> VOI LUT Sequence	(0028,3010)	SQ	Present with single item if a Non-Linear window is to be applied to the Referenced Images	ANAP	USER
>> LUT Descriptor	(0028,3002)	US/SS			
>> LUT Explanation	(0028,3003)	LO			
>> LUT Data	(0028,3006)	OW			
> Window Centre	(0028,1050)	DS	Present if VOI LUT Sequence absent	ANAP	USER
> Window Width	(0028,1051)	DS	Present if VOI LUT Sequence absent	ANAP	USER
> VOI LUT Function	(0028,1056)	CS	Present if VOI LUT Sequence absent SIGMOID if SIGMOID in Image Header LINEAR Otherwise	ANAP	SYSTEM

Table 8.1-24. Softcopy Presentation LUT Module of Created Greyscale Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Presentation LUT Sequence	(2050,0110)	SQ	Taken from image header if present	ANAP	SYSTEM
> LUT Descriptor	(0028,3002)	US			
> LUT Explanation	(0028,3003)	LO			
> LUT Data	(0028,3006)	OW			
Presentation LUT Shape	(2050,0020)	CS	Present if Presentation LUT Sequence Absent IDENTITY INVERSE Seeded from Photometric Interpretation in Image Header, user may subsequently Invert the greyscale	ANAP	SYSTEM

Table 8.1-25. ICC Profile Module of Created Colour Presentation State SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
ICC Profile	(0028,2000)	OB	Standard sRGB IEC61966-2.1 profile	ALWAYS	AUTO

8.1.1.8. Spatial Registration Modules

Table 8.1-26. Spatial Registration Series Module of Created Spatial Registration SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	REG	ALWAYS	AUTO

Table 8.1-27. Frame of Reference Module of Created Spatial Registration SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
----------------	-----	----	-------	-------------------	--------

Frame of Reference UID	(0020,0052)	UI	Frame of Reference IUD for the Registered Reference Coordinate System (RCS) established by this Registration Object	ALWAYS	SYSTEM
Position Reference Indicator	(0020,1040)	LO		EMPTY	

Table 8.1-28. Common Instance Reference Module of Created Spatial Registration SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Reference Series Sequence	(0008,1115)	SQ	Sequence referencing the SOP Instances in this Study which are natively in the Registered RCS Frame of Reference	ALWAYS	SYSTEM
> Series Instance UID	(0020,000E)	UI			
> Referenced Instance Sequence	(0008,114A)	SQ			
>> Referenced SOP Class UID	(0008,1150)	UI			
>> Referenced SOP Instance UID	(0008,1155)	UI			
Studies Containing Other Referenced Instances Sequences	(0008,1200)	SQ	Sequence referencing the SOP Instances from the Frames of Reference transformed by the Registration object to the Registered RCS	ALWAYS	SYSTEM
> Study Instance UID	(0020,000D)	UI			
> Reference Series Sequence	(0008,1115)	SQ			
>> Series Instance UID	(0020,000E)	UI			
>> Referenced Instance Sequence	(0008,114A)	SQ			
>>> Referenced SOP Class UID	(0008,1150)	UI			
>>> Referenced SOP Instance UID	(0008,1155)	UI			

Table 8.1-29. SOP Common Module of Created Spatial Registration SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.66.1	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by InSight System	ALWAYS	AUTO
Instance Creation Date	(0008,0012)	DA	Date of Registration Export	ALWAYS	AUTO
Instance Creation Time	(0008,0013)	TM	Time of Registration Export	ALWAYS	AUTO
Instance Number	(0020,0013)	IS	1	ALWAYS	AUTO

Table 8.1-30. Spatial Registration Module of Created Spatial Registration SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS	1	ALWAYS	AUTO
Content Date	(0020,0023)	DA	Date Registration was performed	ALWAYS	AUTO
Content Time	(0020,0033)	TM	Time Registration was performed	ALWAYS	AUTO
Content Label	(0070,0080)	SH	InSight.Auto InSpect.Rigid	ALWAYS	SYSTEM
Content Description	(0070,0081)	LO	Description from the entity that generated the transform	VNAP	SYSTEM
Creator Name	(0070,0084)	PN	Identifier of the Entity that generated the transform	VNAP	SYSTEM
Registration Sequence	(0070,0308)	SQ	A Sequence of registration Items. Each Item defines a spatial registration of the images referenced in that Item to the Registered RCS established by this SOP instance.	ALWAYS	AUTO
> Frame of Reference UID	(0020,0052)	UI	Identifies the Frame of Reference of the referenced objects	ALWAYS	SYSTEM
> Referenced Image Sequence	(0008,1140)	SQ	The SOP Instances of the objects which are mapped by this registration item	ALWAYS	SYSTEM
>> Referenced SOP Class UID	(0008,1150)	UI			
>> Referenced SOP Instance UID	(0008,1155)	UI			
> Matrix Registration Sequence	(0080,0309)	SQ	A Sequence that specifies one spatial registration. Exactly One Item shall be present	ALWAYS	AUTO
>> Registration Type Code Sequence	(0070,030D)	SQ	Describes the information input into the registration process. One Item will be present	ALWAYS	AUTO
>>> Code Value	(0008,0100)	SH	125024		
>>> Coding Scheme	(0008,0102)	SH	DCM		
>>> Code Meaning	(0008,0104)	LO	Image Content-based Alignment		
>> Matrix Sequence	(0070,030A)	SQ	Specifies one transformation, that registers the Source RCS/images to the Registered RCS. It is expressible as multiple matrices, each in a separate Item of the Sequence. One or more Items shall be included in this Sequence. The Item order is significant and corresponds to matrix multiplication order.	ALWAYS	AUTO
>>> Frame of Reference Transformation Matrix	(3003,00C6)	DS	A 4x4 affine transformation matrix that registers a homogeneous coordinate system A to B. Matrix elements shall be listed in row-major order.		
>>> Frame of Reference Transformation Matrix Type	(0070,030C)	CS	Type of the Frame of Reference Transformation Matrix RIGID RIGID_SCALE AFFINE		

8.1.1.9. IOCM KOS Modules

Table 8.1-31. Key Object Selection Document Series Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	KO	ALWAYS	AUTO
Series Instance UID	(0020,000E)	UI	Generated by InSight System	ALWAYS	AUTO
Series Number	(0020,0011)	IS	1	ALWAYS	AUTO
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ		EMPTY	AUTO

Table 8.1-32. SOP Common Module of Created Key Object Document SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.88.59	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by InSight System	ALWAYS	AUTO

Table 8.1-33. Key Object Document Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS	1	ALWAYS	AUTO
Content Date	(0020,0023)	DA	Date KOS Object created	ALWAYS	AUTO
Content Time	(0020,0033)	TM	Time KOS Object created	ALWAYS	AUTO
Referenced Request Sequence	(0040,A370)	SQ	Single item, details will match those in the Study Module	ALWAYS	SYSTEM
> Study Instance UID	(0020,000D)	UI		ALWAYS	SYSTEM
> Referenced Study Sequence	(0008,1110)	SQ		EMPTY	
> Accession Number	(0008,0050)	SH		ALWAYS	SYSTEM
> Place Order Number / Imaging Service Request	(0040,2016)	LO		EMPTY	
> Filler Order Number / Imaging Service Request	(0040,2017)	LO		EMPTY	
> Requested Procedure Id	(0040,1001)	SH		ALWAYS	SYSTEM
> Requested Procedure Description	(0032,1060)	LO		ALWAYS	SYSTEM
> Requested Procedure Code Sequence	(0032,1064)	SQ		ALWAYS	SYSTEM
>> Code Value	(0008,0100)	SH		ALWAYS	SYSTEM
>> Coding Scheme	(0008,0102)	SH		ALWAYS	SYSTEM
>> Code Meaning	(0008,0104)	LO		ALWAYS	SYSTEM
Current Requested Procedure Evidence Sequence	(0040,A375)	SQ	The Set of Instances affected by the KOS Rejection Note. Single Item	ALWAYS	SYSTEM
> Study Instance UID	(0020,000D)	UI			
> Referenced Series Sequence	(0008,1115)	SQ			
>> Series Instance UID	(0020,000E)	UI			
>> Referenced SOP Sequence	(0008,1199)	SQ			
>>> Reference SOP Class UID	(0008,1150)	UI	At least one item		

>>> Referenced Instance UID	SOP (0008,1155)	UI	SOP Instance affected by Rejection Note		
-----------------------------	-----------------	----	---	--	--

Table 8.1-34. SR Document Content Module of Created IOCM KOS Document SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
Concept Name Code Sequence	(0040,A043)	SQ	Single item identifying the “Key Object Selection Document Title”, taken from DCID 7010, further specialised for an IOCM Rejection Note as below		AUTO
>Code Value	(0008,0100)	SH	113001 113037 113038 113039		SYSTEM
>Coding Scheme Designator	(0008,0102)	SH	DCM		AUTO
>Code Meaning	(0008,0104)	LO	Rejected For Quality Rejected For Patient Safety Incorrect Modality Worklist Entry Data Retention Policy Expired Respectively for each Code Value above		SYSTEM
Continuity of Content	(0040,A050)	CS	SEPARATE	ALWAYS	AUTO
Content Template Sequence	(0040,A504)	SQ	Single item identifying TID 2010, Key Object Selection Root Template		AUTO
>Mapping Resource	(0008,0105)	CS	DCM		AUTO
>Template Identifier	(0040,DB00)	CS	2010		AUTO
Content Sequence	(0040,A730)	SQ	Multiple items as defined in TID 2010, see Rows 2-6 of Table 8.1-35 below		AUTO

Table 8.1-35. TID 2010 Key Object Selection Template.

	NL	Rel with Parent	VT	Concept Name	VM	Condition	Value Set Constraint
1			CONTAINER	DCID 7010 “Key Object Selection Document Title”	1		Root Node as laid out in Table 8.1-34 above
2	>	HAS CONCEPT MOD	CODE	(113011, DCM, “Document Title Modifier”)	1	Iff Key Object Selection Document Title = (113001, DCM, “Rejected for Quality Reasons”)	DCID 7011 “Rejected for Quality Reasons”
3	>	CONTAINS	TEXT	(113012, DCM, “Key Object Description”)	1	Present if user entered text at time of Image Rejection	Text entered by User at time of Image Rejection
4	>	CONTAINS	IMAGE		1-n	At least one of Rows 4-6 will be present	The list of SOP Instances conveyed in the Current Requested Procedure Evidence Sequence (0040,A375)
5	>	CONTAINS	WAVEFORM		1-n		
6	>	CONTAINS	COMPOSITE		1-n		

8.1.1.10. Basic Text Structured Report Modules

Table 8.1-36. Basic Text Structured Report Series Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Modality	(0008,0060)	CS	SR	ALWAYS	AUTO
Series Instance UID	(0020,000E)	UI	Generated by InSight System	ALWAYS	SYSTEM
Series Number	(0020,0011)	IS	1	ALWAYS	AUTO
Referenced Performed Procedure Step Sequence	(0008,1111)	SQ		EMPTY	AUTO

Table 8.1-37. SOP Common Module of Created Basic Text Structured Report SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
SOP Class UID	(0008,0016)	UI	1.2.840.10008.5.1.4.1.1.88.11	ALWAYS	AUTO
SOP Instance UID	(0008,0018)	UI	Generated by InSight System	ALWAYS	AUTO

Table 8.1-38. SR Document General Module of Created SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Instance Number	(0020,0013)	IS	1	ALWAYS	AUTO
Completion Flag	(0040,A491)	CS	COMPLETE	ALWAYS	AUTO
Verification Flag	(0040,A493)	CS	UNVERIFIED VERIFIED	ALWAYS	SYSTEM
Content Date	(0020,0023)	DA	Date underlying Report created	ALWAYS	AUTO
Content Time	(0020,0033)	TM	Time underlying Report created	ALWAYS	AUTO
Verifying Observer Sequence	(0040,A073)	SQ	Single Item if Verification Flag is VERIFIED identifying the individual who Verified the report	ANAP	SYSTEM
> Verifying Observer Name	(0040,A075)	PN	Name of the person who verified the report	ALWAYS	SYSTEM
> Verifying Observer Identification Code Sequence	(0040,A088)	SQ	Zero or One Item	VNAP	SYSTEM
>> Code Value	(0008,0100)	SH		ALWAYS	SYSTEM
>> Coding Scheme	(0008,0102)	SH		ALWAYS	SYSTEM
>> Code Meaning	(0008,0104)	LO		ALWAYS	SYSTEM
> Verifying Organization	(0040,A027)	LO	Organisation to which the Verifying Observer is accountable	ALWAYS	SYSTEM
> Verification DateTime	(0040,A030)	DT	DateTime of the Verification event	ALWAYS	SYSTEM
Author Observer Sequence	(0040,A078)	SQ	Single Item if present identifying the Author of the Report	ANAP	SYSTEM
> Observer Type	(0040,A084)	CS	PSN	ALWAYS	AUTO
> Person Name	(0040,A123)	PN	Name of the person who authored the report	ALWAYS	SYSTEM
> Person Identification Code Sequence	(0040,1101)	SQ	Zero or One Item	VNAP	SYSTEM
>> Code Value	(0008,0100)	SH		ALWAYS	SYSTEM
>> Coding Scheme	(0008,0102)	SH		ALWAYS	SYSTEM
>> Code Meaning	(0008,0104)	LO		ALWAYS	SYSTEM
> Institution Name	(0008,0080)	LO	Institution to which the Author is accountable	VNAP	SYSTEM
> Institution Code Sequence	(0008,0082)	SQ	Empty	EMPTY	

Referenced Request Sequence	(0040,A370)	SQ	Single item, details will match those in the Study Module	ALWAYS	SYSTEM
> Study Instance UID	(0020,000D)	UI		ALWAYS	SYSTEM
> Referenced Study Sequence	(0008,1110)	SQ		EMPTY	
> Accession Number	(0008,0050)	SH		ALWAYS	SYSTEM
> Place Order Number / Imaging Service Request	(0040,2016)	LO		EMPTY	
> Filler Order Number / Imaging Service Request	(0040,2017)	LO		VNAP	SYSTEM
> Requested Procedure Id	(0040,1001)	SH		ALWAYS	SYSTEM
> Requested Procedure Description	(0032,1060)	LO		ALWAYS	SYSTEM
> Requested Procedure Code Sequence	(0032,1064)	SQ		EMPTY	
Performed Procedure Code Sequence	(0040,A372)	SQ		ALWAYS	SYSTEM
>> Code Value	(0008,0100)	SH			
>> Coding Scheme	(0008,0102)	SH			
>> Code Meaning	(0008,0104)	LO			
Current Requested Procedure Evidence Sequence	(0040,A375)	SQ	All Composite SOP Instances in the Study containing this SR. Single Item	ALWAYS	SYSTEM
> Study Instance UID	(0020,000D)	UI	UID of the containing Study		
> Referenced Series Sequence	(0008,1115)	SQ	At least one item		
>> Series Instance UID	(0020,000E)	UI			
>> Referenced SOP Sequence	(0008,1199)	SQ	At least one item		
>>> Reference SOP Class UID	(0008,1150)	UI			
>>> Referenced SOP Instance UID	(0008,1155)	UI			

Table 8.1-39. SR Document Content Module of Created Basic Text Structured Report SOP Instances.

Attribute Name	Tag	VR	Value	Presence of Value	Source
Value Type	(0040,A040)	CS	CONTAINER	ALWAYS	AUTO
Concept Name Code Sequence	(0040,A043)	SQ	Single item identifying the “Diagnostic Imaging Report Title”, taken from DCID 7000		AUTO
>Code Value	(0008,0100)	SH	18748-4		SYSTEM
>Coding Scheme Designator	(0008,0102)	SH	LN		AUTO
>Code Meaning	(0008,0104)	LO	Diagnostic Imaging Report		SYSTEM
Continuity of Content	(0040,A050)	CS	SEPARATE	ALWAYS	AUTO
Content Template Sequence	(0040,A504)	SQ	Single item identifying TID 2005, Transcribed Diagnostic Imaging Report		AUTO
>Mapping Resource	(0008,0105)	CS	DCM		AUTO
>Template Identifier	(0040,DB00)	CS	2005		AUTO
Content Sequence	(0040,A730)	SQ	Multiple items as defined in TID 2005, see Rows 2-7 of Table 8.1-40 below		AUTO

Table 8.1-40. TID 2005 Transcribed Diagnostic Imaging Report.

	NL	Rel with Parent	VT	Concept Name	VM	Condition	Value Set Constraint
1			CONTAINER	BCID 7000 “Diagnostic Imaging Report Document Titles”	1		Root Node as laid out in Table 8.1-39 above
2	>	HAS CONCEPT MOD	CODE	(121058, DCM, “Procedure Reported”)	1-n		Procedure Codes to match Performed Procedure Code SQ (0040,A372)
3	>	HAS CONCEPT MOD	CODE	(122142, DCM, “Acquisition Device Type”)	1-n		DCID 29 “Acquisition Modality
4	>	HAS CONCEPT MOD	CODE	(123014, DCM, “Target Region”)	1-n		DCID 4 “Anatomic Region”
5	>	HAS CONCEPT MOD	CODE	(121049, DCM, “Language of Content Item and Descendants”)	1		DCID 5000 “Languages” { en-GB, RFC5646, “English (UK)” }
6	>	CONTAINS	CONTAINER	From BCID 7001 “Diagnostic Imaging Report Headings”: { 55112-7, LN, “Summary” }	1		
7	>>	CONTAINS	TEXT	From BCID 7002 “Diagnostic Imaging Report Elements” { 121111, DCM, “Summary” }	1		The text of the Report as received from RIS via HL7 messaging.

8.1.2. Usage of Attributes from received IODs

When SOP Instances are received by InDigoX, the source Application Entity and values of certain attributes are registered with the InSight Database if they are present in the SOP Instance, to allow other Applications in the InSight System to access the data without parsing the Stored DICOM Objects. These are as follows:

Table 8.1-41. Attributes Registered with InSight Database on SOP Instance Receipt.

Attribute Name	Tag	Notes
Patient Module		
Patient Name	(0010,0010)	
Patient ID	(0010,0020)	Required
Patient Date of Birth	(0010,0030)	
Patient Sex	(0010,0040)	
General Study Module		
Study Instance UID	(0020,000D)	Required
Study ID	(0020,0010)	
Study Description	(0008,1030)	If Procedure Code Sequence is empty
Study Date	(0008,0020)	
Study Time	(0008,0030)	
Referring Physician Name	(0008,0090)	
Accession Number	(0008,0050)	
Procedure Code Sequence	(0008,1032)	First Item Only
> Code Value	(0008,0100)	
> Code Meaning	(0008,0104)	
Equipment IOD		

Manufacturer	(0008,0070)	
Manufacturer Model Name	(0008,1090)	
General Series IOD		
Series Instance UID	(0020,000E)	Required
Modality	(0008,0060)	
Performing Physicians' Names	(0008,1050)	First Value Only
Body Part Examined	(0018,0015)	
Series Number	(0020,0011)	
Series Description	(0008,103E)	
Patient Position	(0018,5100)	
Series Date	(0008,0021)	
Series Time	(0008,0031)	
Laterality	(0020,0060)	(0020,0062) if present in Specialised Image Module, or Functional Groups (5200,9229) / (5200,9230)
Request Attribute Sequence	(0040,0275)	
> Requested Procedure Id	(0040,1001)	
> Requested Procedure Code SQ	(0032,1064)	
>> Code Value	(0008,0100)	
>> Code Meaning	(0008,0104)	
>> Coding Scheme Designator	(0008,0102)	
> Reason for Requested Procedure	(0008,1002)	
> Reason for Requested Procedure Code Sequence	(0040,100A)	
>> Code Value	(0008,0100)	
>> Code Meaning	(0008,0104)	
>> Coding Scheme Designator	(0008,0102)	
> Scheduled Procedure Step Id	(0040,0009)	
> Scheduled Procedure Step Description	(0040,0007)	
Multiframe Functional Groups Module		
Shared or Per-Frame Functional Groups Sequence	(5200,9229) (5200,9230)	
> Frame Anatomy Sequence	(0020,9071)	
>> Laterality	(0020,9072)	'Both' if present with different values for different frames
General Image Module		
Image Type	(0008,0008)	First 3 values recorded
Acquisition Date	(0008,0022)	
Acquisition Time	(0008,0032)	
Content Date	(0008,0023)	
Content Time	(0008,0033)	
Instance Number	(0020,0013)	
Reference Image Sequence	(0008,1140)	Required for Presentation State SOP Classes
> Reference SOP Instance	(0008,1155)	
SOP Common		
SOP Class UID	(0008,0016)	
SOP Instance UID	(0008,0018)	
Multiframe IOD		
Number of Frames	(0028,0008)	
Frame of Reference IOD		
Frame of Reference UID	(0020,0052)	
Image Pixel IOD		
Bits Stored	(0028,0101)	Required if Pixel Data Present
Signed Data	(0028,0103)	Required if Pixel Data Present
Rows	(0028,0010)	
Columns	(0028,0011)	
Pixel Data	(07FE,0010)	Required for Image Storage SOP Classes

Image Plane IOD		
Image Orientation	(0020,0037)	
Image Position	(0020,0032)	
Slice Thickness	(0018,0050)	
Slice Location	(0020,1041)	
Imager Pixel Spacing	(0018,1164)	Used to calculated pixel size in conjunction with given or calculated magnification factor
Estimated Radiographic Magnification Factor	(0018,1114)	
Distance Source to Patient	(0018,1111)	
Distance Source to Detector	(0018,1110)	
Pixel Spacing	(0028,0030)	
Modality LUT IOD		
Rescale Intercept	(0028,1052)	
Rescale Slope	(0028,1053)	
VOI LUT IOD		
Window Centre	(0028,1050)	Only first value is recorded in Database
Window Width	(0028,1051)	Only first value is recorded in Database
Cine IOD		
Cine Rate	(0018,0040)	
CR / DX / MG Modules		
View Position	(0018,5101)	Will use Code in View Code Sequence (0054,0220) in preference if present in Specialised Image Module
View Code Sequence	(0054,0220)	
> Code Value	(0008,0100)	
> View Modifier Code Sequence	(0054,0222)	
>> Code Value	(0008,0100)	
MR Image Module		
Temporal Position Identifier	(0020,0100)	
Number of Temporal Positions	(0020,0105)	

8.1.3. Attribute Mapping

The InSight System is highly configurable when mapping Real World information to values received in SOP Instances and from information received over an HL7 (or other) data feed. The Data Feed is configured to take items from various places in the HL7 (or other) protocol and map these to InSight Database fields representing Real World Hierarchy Levels such as Visit, Admission, Requested Procedure, Scheduled Procedure Step etc.

Each Remote Application Entity which can perform Worklist Queries has its own section of configuration in the InSight System which specifies how the Real World information is then mapped to various DICOM Attributes for the CFind Request and Responses. In particular the usage of Study ID, Accession Number, and Requested Procedure Id and Scheduled Procedure Step Id in the Request Attribute Sequence is configurable.

Each Remote Application Entity which can generate and send SOP Instances to InDigoX also has individual configuration on the InSight System which records where that modality places the pieces of Real World information so the fields detailed in **Table 8.1-41** can be mapped to the real world data hierarchy identifiers in the InSight Database. This same mapping is used when updating volatile information when sending SOP Instances back to Remote Application Entities via Inquire to ensure that the Real World information is conveyed in the expected DICOM Attributes for the given target Application Entity.

8.1.4. Coerced / Modified fields

When SOP Instances are sent by InQuire, certain fields may be different to those as they were received by InDigoX. The changes will be in response to altered hierarchy and real-world information as received by the System Information Feed (from the Institution RIS or otherwise), or as entered by Administrative Users via the InSight System tools. When such changes occur, they are logged in the InSight System.

Table 8.1-42. Fields Updated.

Field	Tag
Patient Name	(0010,0010)
Patient ID	(0010,0020)
Patient Date of Birth	(0010,0030)
Patient Sex	(0010,0040)
Other Patient ID	(0010,1000)
Study Instance UID	(0020,000D)
Study ID	(0020,0010)
Study Date	(0008,0020)
Study Time	(0008,0030)
Accession Number	(0008,0050)
Referring Physician Name	(0008,0090)
Study Description	(0008,1030)
Procedure Code Sequence	(0008,1032)
> Code Value	(0008,0100)
> Code Meaning	(0008,0104)
> Coding Scheme Designator	(0008,0102)
> Coding Scheme Version	(0008,0103)
Physician of Record Names	(0008,1048)
Performing Physician Name	(0008,1050)
Reading Physician Names	(0008,1060)
Series Instance UID	(0020,000E)
Body Part Examined	(0018,0015)
SOP Instance UID	(0008,0018)
Request Attribute Sequence	(0040,0275)
> Scheduled Procedure Step Id	(0040,0009)
> Requested Procedure Id	(0040,1001)
> Requested Procedure Code SQ	(0032,1064)
>> Code Value	(0008,0100)
>> Code Meaning	(0008,0104)
>> Coding Scheme Designator	(0008,0102)
>> Coding Scheme Version	(0008,0103)

8.2. Data Dictionary of Private Attributes

The InSight DICOM Application Entities detailed in this document do not generate any Private Attributes

8.3. Coded Terminology and Templates

8.3.1. Private Code Definitions

The InSight System receives Requested Procedure and Scheduled Procedure Step Codes from the Institution Information System data feed. Often this data feed does not contain a meaning for the Code, so the InSight

Database has reference data to supply a Code Meaning for each Code Value used by the Institution. When generating responses to Modality Worklist Queries, it is the Code Value received from the Information feed along with the configured Code Meaning that are passed on to the requesting Application Entity in the Requested Procedure Code and Scheduled Procedure Code Sequence fields of the query responses. The InSight System has a configuration item to record the Designator of the codes used by an Institution which will be used if known; otherwise the Coding Scheme Designator will be given as “INSIGNIA PRIVATE”.